



The Open Dentistry Journal

Content list available at: <https://opendentistryjournal.com>



RESEARCH ARTICLE

Investigating the Effect of Different Metal Sheets on Reducing Radiation Behind Intraoral Digital Phosphor Plates During Intraoral Radiography using Gray Value

Mojdeh Mehdizadeh¹, Mohammad Bagher Tavakoli² and Farida Ghazanfari Moghaddam^{3,*}

¹Department of Oral and Maxillofacial Radiology, Dental Implant Research Center, Dental Research Institute, School of Dentistry, Isfahan University of Medical Sciences, Isfahan, Iran

²Department of Medical Physics and Medical Engineering, School of Medicine, Isfahan University of Medical Sciences, Isfahan, Iran

³Dental Students Research Committee, Department of Oral and Maxillofacial Radiology, School of Dentistry, Isfahan University of Medical Sciences, Isfahan, Iran

Abstract:

Purpose:

To assess the efficacy of metal sheets with different thicknesses on reducing the radiation behind the photostimulable phosphor plate (PSP) during intraoral periapical examinations.

Materials and Methods:

In this study, a phantom head was used to investigate the effect of using metal sheets of aluminum, stainless steel, and copper with three thicknesses of 0.5, 0.75 and 1mm on reducing the radiation behind PSP. Images were acquired at 66 kVp 8 mA, and 0.16 s using the long-cone paralleling technique. The images were saved and exported to DICOM format without any post-processing. Then, they were transferred to an image processing software (Mimics, Materialize, Leuven, Belgium), and their mean gray values (MGV) were determined. The acquired data were statically analyzed for accessing the significant difference in groups means using ANOVA, and the means of groups were compared using Tukey's test procedure.

Results:

The MGV of the second PSP differed significantly from those PSPs slotted with various metals ($p < 0.001$). The MGV for lead and stainless steel at 0.5 mm thickness was insignificant ($p = 0.852$), but differed significantly from other metals. The MGV for PSPs with 0.75 mm stainless steel and 1 mm copper slots were varied significantly from those of all other PSP and metals. The 1 mm copper group was significantly different from all other groups ($p < 0.001$).

Conclusion:

Using the mean gray value of the PSP, the use of various metal sheets of different thicknesses could effectively reduce the radiation behind the PSPs during periapical radiographs.

Keywords: Radiation protection, Dental, Digital radiography, Diagnostic imaging, X-ray, Phantom head.

Article History

Received: July 25, 2020

Revised: November 26, 2020

Accepted: November 27, 2020

1. INTRODUCTION

Recent advances in radiology techniques have introduced substantial diagnostic benefits in dentistry [1]. In X-ray radiology, despite low dose received by a patient during radio-

graphy, there are still concerns about the carcinogenicity of X-rays and exposure to ionizing X-rays. Exposing to X-ray radiation is always can be accompanied by some risks [2]. However, various protective devices and techniques have been used to reduce the levels of radiation received by patients.

The development of digital radiography has led to many improvements in the field of diagnostic imaging. Features such as the wider amplitude of radiation and greater sensitivity of

* Address correspondence to this author at the Dental Students Research Committee, Department of Oral and Maxillofacial Radiology, School of Dentistry, Isfahan University of Medical Sciences, Isfahan, Iran; E-mail: f_gh_moghaddam@yahoo.com

digital receptors and sensors have reduced the amount of radiation that patients are exposed [3]. Digital radiographic sensors have two broad categories of photostimulable phosphor plates (PSPs) and silicon devices. The PSP systems do benefit from being user-friendly, compared to conventional intraoral radiology films [4].

In conventional film-based intraoral radiography, the amount of radiation passing through a PSP is reduced by a lead foil. This lead foil, which is a protective metal sheet plays two major roles in dental x-ray films. First, it reduces the transmitted radiation and the absorbed dose by the tissue behind the film envelope. Second, it prevents backscatter radiation from the tissues to maintain image quality [5, 6]. However, due to shorter exposure time for image acquisition, lead foils are rarely used in digital radiography. However, the necessity of shielding materials still cannot be neglected, based on the “as low as reasonably achievable, (ALARA)” principle [7].

On the other hand, there have been many concerns over lead toxicity over the past years, and lead poisoning in both children and adults has been well documented [8]. There are also reports of the need to modify the criteria due to the corrosion of the lead sheet when used as a structural shield [9]. Lead foils, when outside an envelope, often come direct contact with fingers and mouth tissues and may lead to deleterious effects [10]. On the other hand, concerns about lead environmental pollution and its proper disposals, have severely restricted its uses. The EU directive “Restriction on the Use of Hazardous Certain Materials” for electrical and electronic equipment has forbidden the use of lead in electrical appliances since July 1, 2006. Therefore, lead-free products in healthcare and industrial applications are in high demand [11].

Much research had been done on the use of non-lead metals to reduce the role of lead protectors. However, the use of other metal sheets as an alternative to lead foils requires

more scientific attention. The purpose of this study was to evaluate the effect of different metals, including stainless steel, copper and aluminum with different thicknesses, on reducing radiation exposure behind photostimulable phosphor plates (PSPs) during periapical intraoral examinations.

2. MATERIALS AND METHODS

Phantom head (DXTTR III X-ray Trainer) was used for taking the required images in all experiments. The phantom head consisted of an adult human skull with jaws and normal teeth covered by plastic material. The plastic materials were composed of substances that were equivalent to actual tissue in terms of absorption and attenuation of radiation. In order to investigate the effect of different metals on radiation behind PSPs, three common metal sheets, including aluminum, stain less steel, and copper with thicknesses of 0.5, 0.75 and 1.0 mm were prepared.

As ISO recommends a film packet thickness below 2.0 mm, the thicknesses of our packet, including the PSP and metal sheet, were within the recommended operational thickness [12]. The metal sheets were similar in size to the PSP Vista Scan phosphor plate system (Dürr Dental, Beitigheim - Bissingen, Germany), size 2, 40.0 mm × 30.0 mm. Since lead foils are commonly used in conventional radiography films, this type of foils was also used as a group for comparison.

The back of each PSP was marked with different colors, a blue arrow for the first PSP and a green arrow for the second PSP, to differentiate the PSPs. Also, in order to differentiate radiographs, for the first PSP the dot was placed in the occlusal and for the second PSP the dot was placed in the apical. Two fixed PSPs were used for all the experiments. The lead foil in the E Speed Carestream Kodak Films was then inserted inside the black paper and plastic cover of E Speed Carestream Kodak Films and placed between the PSPs and they were all placed inside a plastic envelope (Fig. 1).

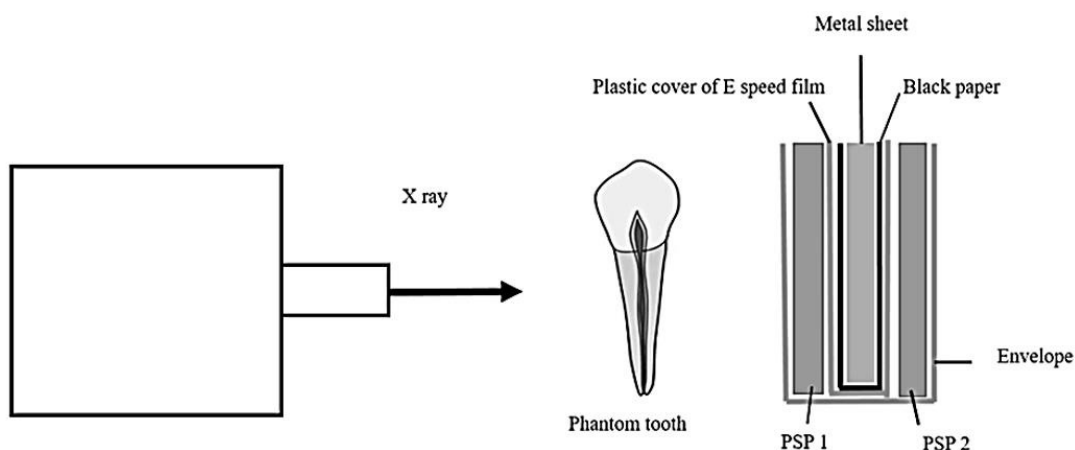


Fig. (1). A schematic view showing the position of various metals between the PSPs.

To help positioning the image receptor and to reproduce the parallel technique, the region of lower mandibular molars was selected from lingual cusp of first left premolar to the mesial of third molar. Initially, PSPs alone were inserted inside the plastic envelope. Using a 30 cm long cylindrical collimator equipped with a rectangular PID (Dentsply / Rinn XCP Corporation, Elgin, IL, USA), and a film holder (Rinn-Endo-Ray) was set at a distance 2 cm from the phantom face. For acquiring the images the vertical and horizontal angulations were set to 0° and 90°, respectively. In addition, the object-detector distance of 1 cm were used throughout the experiments (Fig. 2).



Fig. (2). Image of the phantom head (DXTR III X-Ray Trainer), composing of tissue-equivalent materials, and positioning of the tube.

Radiation conditions were set at 66 kVp at 8 mA and 0.16 s. Imaging was performed by a dental X-ray unit (Planmeca OY, Helsinki, Finland) and the images were immediately scanned with Scanora 5.0 software (Sorodex, Helsinki, Finland). After saving, all of the image were exported to DICOM format without any post-processing. Then, they were transferred to mimics software (Mimics, Materialize, Leuven, Belgium) in order to measure the mean gray value of each PSPs. In an 8-bit grayscale image, each pixel may take a value from 0 to 256. A 0 value represents a black pixel (minimum density) and 256 represents a white pixel (maximum density).

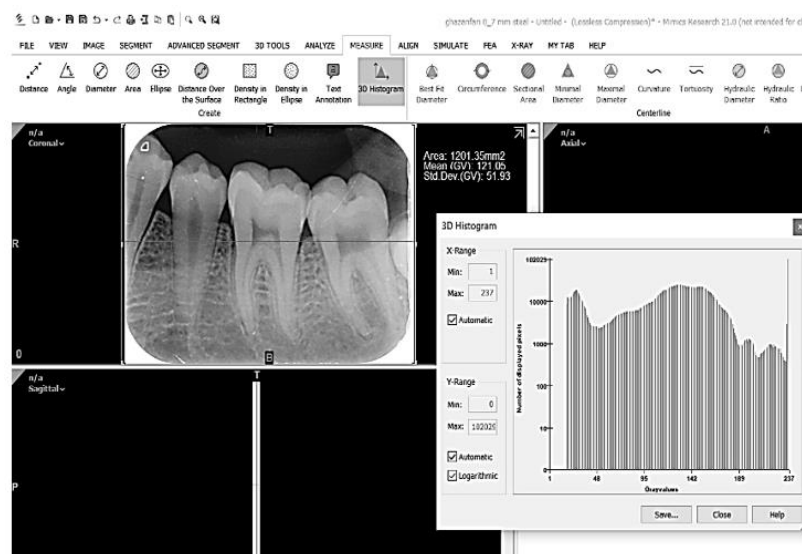


Fig. (3). The histogram and mean gray value of the total PSP image on Mimics software.

The mean gray value of the region of interest that was equal to the total area of PSP, was measured with the rectangular density region icon of the software. The histogram of each image was also evaluated. The histogram graphically displays the distribution of pixels amongst the grayscale values. The x-axis shows the gray value (from 0 to 256), the y-axis shows their frequency in the image (Fig. 3). The same procedure was applied to the other metal sheets used in the study. All experiments were repeated 10 times and immediately scanned.

2.1. Data Analysis

To investigate any significant difference between the mean gray values of the groups, one-way ANOVA, with 11 groups and 10 replicates for each group, was performed. Initially, the assumption for normality of data for each group, required for the ANOVA test, was verified by the Kolmogorov-Smirnov test. Then, using Tukey's test, all experiments were compared in pairs for each group of the second PSP. All statistical analyses were performed using the SPSS statistic software, v.22 package (IBM corp, formerly SPSS Inc, Chicago, USA), based on 95% confidence and a margin error of 0.5%.

3. RESULTS

Typical images and histograms of the second images of different metals are shown in Fig. (4). The histogram of the second images in the non-metal group had a uniform distribution with a peak mean gray value of 122.82 locating in the mid region. The distribution of the gray values in the histogram of the metal groups is skewed to the right, indicating more dark pixels in these images. Comparison of the histograms of different groups indicated that as the atomic number increased from aluminum to stainless steel (iron) and to copper, and also by increasing the metal thickness from 0.5 mm to 1mm, the frequency of the light gray shades decreased and the dark gray shades increased. For example, the mean gray value 94 for the lead group was 94.88 and for the 1mm Cu group it was 66.88.

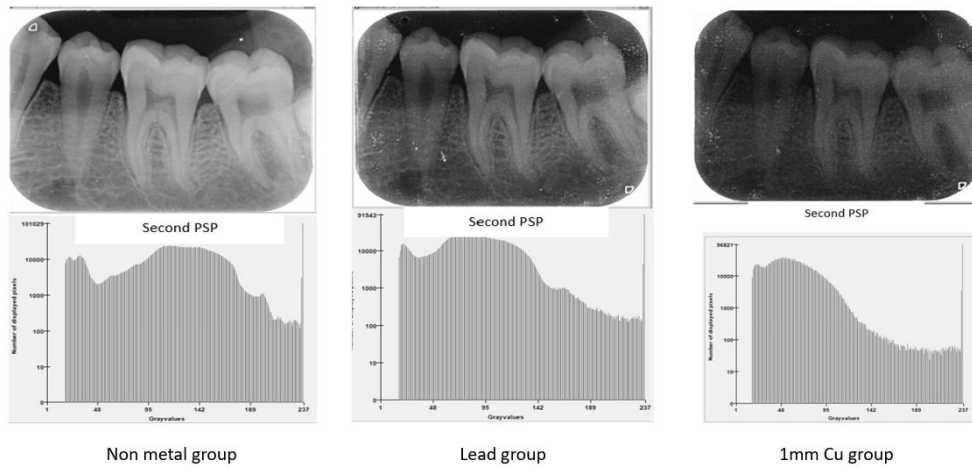


Fig. (4). Typical radiograph images and histograms of the second PSP in the non-metal, lead and 1 mm copper group.

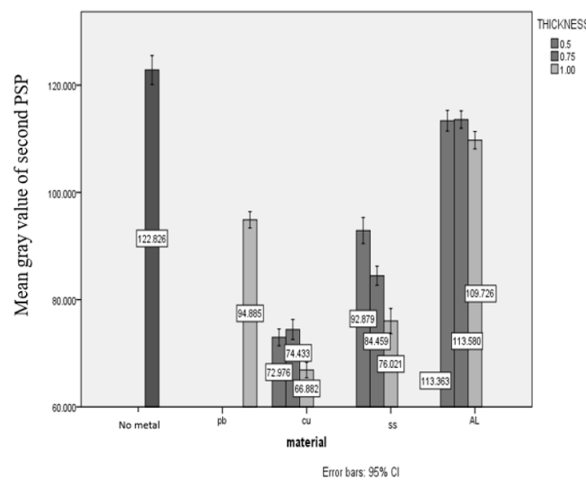


Fig. (5). Mean and 95% confidence intervals of mean gray values in the second PSP based on thickness and type of metal.

Table 1. Descriptive indicators of mean gray value in the second PSP.

Groups	n	Mean	Std. Deviation	Std. error	95% Confidence Interval for Means		Min.	Max.
					Lower Bound	Upper Bound		
No metal	10	122.82	3.77	1.19	120.12	125.52	117.46	129.57
Pb	10	94.88	2.12	0.67	93.36	96.40	91.59	97.96
Cu 0.5mm	10	74.97	2.19	0.69	71.40	74.54	70.17	76.03
Cu 0.75mm	10	72.43	2.59	0.82	72.57	76.28	71.68	78.57
Cu 1mm	10	66.88	2.00	0.63	65.44	68.31	63.22	69.86
SS 0.5mm	10	92.87	3.40	1.07	90.44	95.31	86.02	96.55
SS 0.75mm	10	84.45	2.48	0.78	82.67	86.23	80.09	88.81
SS 1mm	10	76.02	3.28	1.03	73.66	78.37	72.75	82.00
Al 0.5mm	10	114.36	2.69	0.85	111.43	115.29	110.15	116.91
Al 0.75mm	10	113.58	2.25	0.71	111.96	115.19	111.34	118.69
Al 1mm	10	109.72	2.26	0.71	108.10	111.34	106.26	113.57

Pb, Cu, SS, Al stands for lead, copper, stainless steel, aluminum, respectively.

The descriptive statistics for MGV data for the images in the second PSP are presented in Table 1 and graphical comparison for the calculated means with their corresponding

95% confidence intervals is presented in Fig. (5). The highest mean is 122.82 for no metal PSP which indicates the addition of any metal will cause a reduction in MGV. Also, with an

increase in the thickness of the metals, the MGV of the second PSP decreased. The minimum MGV belonged to the copper group with a thickness of 1 mm with MGV = 66.88. A lower MGV indicates a darker image and when an image is darker, less radiation passes through a metal between the PSPs. Thus, as Table 1 indicates, the lowest amount of radiation passed when copper with a thickness of 1.0 mm was used. The average MGV for copper groups was 70, which was lower than other metal groups. The minimum MGV was 63.22 for 1.0 mm copper. The maximum MGV appeared for PSPs having no metal that was equal to 129.57.

The results of the ANOVA test the experimental groups are given in Table 2. The table indicates that the groups have significantly different means ($p < 0.001$). To find out which groups significantly differed from others, the comparison of the means was made using Tukey's test. The results of Tukey's test are presented in Table 3. The table indicates that, in the comparison between the images of the second PSP, MGV of the non-metallic group was significantly different from all other groups containing metals ($p < 0.001$). The groups for aluminum having different thicknesses were not significantly different from each other ($p = 0.067$), but they were significantly different from the other groups. Lead and stainless steel with 0.5 mm thickness were not significantly different ($p = 0.852$), but they were significantly different from other groups. The 0.75 mm stainless steel group was significantly different from all other groups ($p < 0.001$). The 1 mm stainless steel group, copper 0.5 mm and copper 0.75 mm were not significantly different from each other ($p = 0.307$), but they were significantly different from other groups. The 1 mm copper group was significantly different from all other groups ($p < 0.001$). (Table 3).

Table 2. ANOVA table for the MGV data of the second image for 11 groups.

Source	Degrees of Freedom	Sum of Squares	MS	F value	p value
Groups	10	42962.4	4296.2	52.15	0.000
Error	139	11450.2	82.4	-	-
Total	149	54412.6	-	-	-

4. DISCUSSION

Features such as a higher dynamic range and greater sensitivity of digital sensors can reduce the amount of radiation to which patients are exposed. This perception was the main reason for the recent move from conventional to digital radiography in dentistry [13]. Digital systems apply lower doses compared to conventional radiography and use no protective materials such as lead foil. Therefore, it is necessary to examine the radiation behind PSPs to confirm the need for protective materials in digital systems.

In this study, we used the mean gray value of the second PSP for evaluating the reduced radiation by placing metal sheets behind the PSP. Ten different groups of metals with different thickness and one group with no metals were used for this investigation. The mean gray value of the second images for each group were determined and compared. Based on the findings, the use of metal reduced the mean gray value and

reduced the radiation absorption of the second PSP.

Table 3. Categorize similar and different groups for the second PSP based on the Tukey method.

PSP Second Group	Subsets ($p = 0.05$)					
	1	2	3	4	5	6
Cu 1mm	66.88	-	-	-	-	-
Cu 0.5mm	-	72.97	-	-	-	-
Cu 0.75mm	-	74.43	-	-	-	-
SS 1mm	-	76.02	-	-	-	-
SS 0.75mm	-	-	84.46	-	-	-
SS 0.5mm	-	-	-	92.88	-	-
Pb	-	-	-	94.89	-	-
Al 1mm	-	-	-	-	109.73	-
Al 0.5mm	-	-	-	-	113.36	-
Al 0.75	-	-	-	-	113.58	-
No metal	-	-	-	-	-	122.83
sig	1.000	.307	1.000	.852	.067	1.000

There were no significant differences between the MGV of 1 mm aluminum, 0.5 mm aluminum and 0.75 mm aluminum, but they were significantly different from the other groups. There was no significant difference between a lead and stainless steel in 0.5 mm but these two groups were significantly different from other groups. In fact, the effect of 0.5 mm stainless steel in reducing radiation was similar to lead foil in E Speed Carestream Kodak Films (atomic number 82 and 0.1 mm thickness). The 0.75 mm steel was significantly different with all other groups. The 1 mm steel, 0.5 mm copper and 0.75 mm copper groups did not differ significantly from each other, but these three groups were significantly different from the other groups. The 1 mm copper group was different from all other groups.

The most reduction of MGV was in the 1 mm copper group. As the atomic number of the metals, their thickness and the k-layer increased, the x-ray absorption was also increased, and the MGV decreased, and the image was darker. The histogram of gray value of the images in the PSP in the metal-free group was generally uniform with gray peaks locating in the middle region, but in the second images of the other groups, with increasing atomic number and metal thickness, amount of MGV decreased and the distribution of dark gray shades increased. In the second image, the peak mean gray moved to the right indicating darker images.

The causes of darkening of the second PSP image were:

- Some are initial X-rays photons pass through the phantom tooth and cause the image.
- Scattered X-ray from the metal [14].
- The energy released from excited electrons on the surface of the metal due to the absorbing radiation received by the digital sensor.
- The preprocessing of the device. Because even in suboptimal exposure, digital images are rarely very clear. The image preprocessing process usually involves automatic data leveling [15]. Therefore, in this method, using the mean gray shade, it was

concluded that increase in atomic number and increase in the thickness of the metal sheet, the second PSP image became darker.

Nejaim *et al.* [16] using a thermo-luminescent dosimeter reported on the effect of lead foil in a full mouths digital intra-oral radiography for reducing various organ doses. Consequently, lead foil reduced the doses to approximately 32% in the PSP system. Although the two study results cannot be directly compared, this study results support their findings for shielding effects by lead foil in the PSP system.

In a study by Nagasaka *et al.* [17], tungsten sheets it was indicated that this sheet adequately shielded the back radiation of the PSP. They reported that the doses behind the PSP without protective material were no different from behind a conventional film with lead foil. This result indicates that the PSP itself has the effect of reducing the equivalent of using a film with lead foil. In addition, the doses behind the PSP were more reduced by lead foil and tungsten sheets and this was significantly different in all areas compared to non-shielded PSPs. They concluded that tungsten sheets as an alternative shielding agent that could significantly reduce the radiation dose behind PSP. However, tungsten is a relatively high cost metal, but the sheets can be used several times. In our study, we used metals that are readily available, less expensive, and are available in different thicknesses. In addition, all of these sheets can be autoclaved, sterilized without alteration, and increases the rigidity of the PSP for bending in a mouth. ISO recommends that the thickness of a film package be less than 2 mm. Although the PSP package with metal sheets did not exceed this recommended value, patient inconvenience should be assessed.

CONCLUSION

The results of this study based on mean gray values of the images behind metal sheets indicated that:

1. The addition of lead and other metal sheets to PSP significantly reduced the amount of radiation.
2. Radiation reduction was decreased by an increase in atomic number and thickness of the metals.
3. Copper with 1.0 mm thickness resulted in the lowest radiation reduction.

ETHICS APPROVAL AND CONSENT TO PARTICIPATE

This study was approved by the Ethics Committee of Isfahan University of Medical Sciences, Iran. (IR.MUI.RESEARCH.REC.1398.696).

HUMAN AND ANIMAL RIGHTS

No Animals were used in this research. All human research procedures were followed in accordance with the ethical standards of the committee responsible for human experimentation (institutional and national), and with the Helsinki Declaration of 1975, as revised in 2013.

CONSENT FOR PUBLICATION

Not applicable.

AVAILABILITY OF DATA AND MATERIALS

The data that support the findings of this study are available from the corresponding author, [F.G.M], upon reasonable request.

FUNDING

This project was supported by Isfahan University of Medical Sciences, Isfahan, Iran.

CONFLICT OF INTEREST

The authors declare no conflict of interest, financial, or otherwise.

ACKNOWLEDGEMENTS

Declared none.

REFERENCES

- [1] Ludlow JB, Davies-Ludlow LE, White SC. Patient risk related to common dental radiographic examinations: the impact of 2007 International Commission on Radiological Protection recommendations regarding dose calculation. *J Am Dent Assoc* 2008; 139(9): 1237-43.
- [2] Mehdizadeh M, Bagherieh S. Evaluation of relationship between exposure parameters and maxillofacial bone quality with salivary glands absorbed dose in cone beam computed tomography imaging. *J Contemp Dent Pract* 2018; 19(5): 568-73. [<http://dx.doi.org/10.5005/jp-journals-10024-2300>] [PMID: 29807968]
- [3] Alcaraz M, Navarro C, Vicente V, Canteras M. Dose reduction of intraoral dental radiography in Spain. *Dentomaxillofac Radiol* 2006; 35(4): 295-8. [<http://dx.doi.org/10.1259/dmfr/26405790>] [PMID: 16798929]
- [4] Poppe B, Looe HK, Pfaffenberger A, *et al.* Radiation exposure and dose evaluation in intraoral dental radiology. *Radiat Prot Dosimetry* 2007; 123(2): 262-7. [<http://dx.doi.org/10.1093/rpd/nc113>] [PMID: 16971397]
- [5] Price C. An evaluation of lead foil in dental X-ray film packets. 1. Factors affecting the intensity of back-scattered radiation and the effect of this radiation on radiographic contrast when density is allowed to increase. *Br Dent J* 1972; 133(7): 300-4. [<http://dx.doi.org/10.1038/sj.bdj.4802911>] [PMID: 4509449]
- [6] Price C. An evaluation of lead foil in dental X-ray film packets. 2. The effect of back-scattered radiation on radiographic contrast when the density is maintained at an optimum level. *Br Dent J* 1972; 133(8): 343-6. [<http://dx.doi.org/10.1038/sj.bdj.4802917>] [PMID: 4510027]
- [7] Kaeppler G, Dietz K, Herz K, Reinert S. Factors influencing the absorbed dose in intraoral radiography. *Dentomaxillofac Radiol* 2007; 36(8): 506-13. [<http://dx.doi.org/10.1259/dmfr/32903218>] [PMID: 18033949]
- [8] Healey N. Lead toxicity, vulnerable subpopulations and emergency preparedness. *Radiat Prot Dosimetry* 2009; 134(3-4): 143-51. [<http://dx.doi.org/10.1093/rpd/ncp068>] [PMID: 19398444]
- [9] Schick DK, Casey RN, Sim LH, Siddle KJ. Corrosion of lead shielding in a radiology department. *Australas Radiol* 1999; 43(1): 47-51. [<http://dx.doi.org/10.1046/j.1440-1673.1999.00611.x>] [PMID: 10901870]
- [10] Tsuji LJS, Fletcher GG, Nieboer E. Dissolution of lead pellets in saliva: a source of lead exposure in children. *Bull Environ Contam Toxicol* 2002; 68(1): 1-7. [<http://dx.doi.org/10.1007/s00128-001-0211-y>] [PMID: 11731824]
- [11] Directive 2002/95/EC of the European Parliament and of the Council of 27. On the restriction of the use of certain hazardous substances in electrical and electronic equipment. *Off J Eur Union* 2003; 46
- [12] International Organization for Standardization (ISO). ISO 3665: 2011E Photography Intra-oral dental radiographic film and film packets-

- Manufacture Specification. 3rd ed. 2011.
- [13] Hart D, Hillier M, Shrimpton P. on Doses to patients from radiographic and fluoroscopic X-ray imaging procedures in the UK Chilton: Health Protection Agency Centre for Radiation, Chemical and Environmental Hazards 2010.
- [14] Araki K, Kanda S, Toyofuku F. A study of the effects of lead foil in dental X-ray film packets on radiographic image quality. *Dentomaxillofac Radiol* 1993; 22(4): 179-82. [<http://dx.doi.org/10.1259/dmfr.22.4.8181643>] [PMID: 8181643]
- [15] White SC, Pharoah MJ. *Oral radiology: principles and interpretation.* Elsevier Health Sciences 2018.
- [16] Nejaim Y, Silva AI, Brasil DM, Vasconcelos KF, Haiter Neto F, Boscolo FN. Efficacy of lead foil for reducing doses in the head and neck: a simulation study using digital intraoral systems. *Dentomaxillofac Radiol* 2015; 44(8):20150065 [<http://dx.doi.org/10.1259/dmfr.20150065>] [PMID: 26084474]
- [17] Nagasaka T, Izumi M, Gotoh K, *et al.* Use of tungsten sheet as an alternative for reducing the radiation dose behind the digital imaging plate during intra-oral radiography. *Dentomaxillofac Radiol* 2018; 48(1):20180161 [<http://dx.doi.org/10.1259/dmfr.20180161>] [PMID: 30028195]

© 2020 The Author(s). Published by Bentham Open.



This is an open access article distributed under the terms of the Creative Commons Attribution 4.0 International Public License (CC-BY 4.0), a copy of which is available at: <https://creativecommons.org/licenses/by/4.0/legalcode>. This license permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.