









The Open Dentistry Journal

Content list available at: <https://opendentistryjournal.com>



SYSTEMATIC REVIEW

Accuracy in the Marginal Adaptation and/or Internal Adaptation of Full-coverage Fixed Prostheses Made with Digital Impressions and Conventional Impressions: A Systematic Review

María Cajas-Guamán¹ , María Cabrera-Toro^{1*} , Jaime Astudillo-Ortiz¹ , Yulissa Abad-Salinas¹ , Daniela Astudillo-Rubio¹  and Bolívar Delgado-Gaete² 

¹Postgraduate Oral Rehabilitation and Implant-Assisted Prosthesis, Faculty of Dentistry, University of Cuenca, Cuenca 010107, Ecuador

²School of Dentistry, Department of Prosthodontics, Catholic University of Cuenca, Cuenca, Ecuador

Abstract:

Aim:

The study aimed to verify compliance of the systematic reviews with the requirements established by the scientific community and demonstrate the validity and reliability of the systematic reviews conducted on the accuracy (marginal adaptation and/or internal adaptation) of the full-coverage fixed prostheses made with digital impressions versus conventional impressions.

Methods:

A search was performed for systematic reviews in three electronic databases, PubMed, Scopus, and Web of Science, as well as in the gray literature. In the search strategy, medical subject heading (MeSH) words were used in PubMed, and free terms were used for the titles and abstracts of each article. Each keyword was separated by the Boolean operator OR and later combined with the Boolean operator AND. Six systematic reviews were included for qualitative synthesis. To assess the methodological quality of the included systematic reviews, the AMSTAR 2 tool was used.

Results:

The search yielded 131 studies, of which 78 remained after removing duplicates. The title and abstract of each chosen study were assessed, and 22 articles were included for full-text reading. Finally, six studies were included, of which three studies were considered to have low confidence, while the other three were considered to have critically low confidence. In addition, the six SRs evaluated the adaptation or marginal fit, while only three studies measured internal adaptation.

Conclusion:

The use of digital impressions in single fixed prostheses maintains a marginal level within the limit of clinical acceptability; however, the methodological quality of systematic reviews is poor, according to the AMSTAR 2 tool.

Keywords: Marginal fit, Internal fit, Conventional impressions, Digital impressions, Fixed prostheses, Systematic review.

Article History

Received: June 20, 2022

Revised: January 10, 2023

Accepted: February 16, 2023

1. INTRODUCTION

“Computer-aided design and manufacturing” (CAD/CAM) has been used in the preparation of dental restorations, especially crowns and ceramic fixed prostheses, since the 1980s [1 - 4]. It is believed that fixed dental prostheses, fabricated from intraoral digital impressions, have several notable advantages over those obtained through conventional impressions [5 - 9]. For instance, digital impressions better pre-

vent errors of accuracy in the restoration margins than conventional impressions [10]. In addition, the general operating cost of the procedure and the clinical work time are reduced compared to conventional impressions [11 - 16].

A growing number of fixed prostheses are made using intraoral digital impressions, so this technique has become a fundamental part of digitalization in prosthodontics [17 - 21]. A good-quality fixed prosthesis that ensures treatment longevity depends on the marginal accuracy and internal fit between the abutment and the restoration [9, 22, 23]. The most common indicators of poorly adjusted restorative margins [24 -

* Address correspondence to this author at the Faculty of Dentistry, University of Cuenca, Cuenca 010107, Ecuador; Tel.: +593 0982827326; E-mail: mmct_17@hotmail.com

31] are cement dissolution, plaque retention, periodontal problems, such as increased gingival inflammation and probing depth [32], dental hypersensitivity, and caries [33, 34]. The use of intraoral scanners has been introduced to minimize microadaptation errors and subsequent problems that conventional impression techniques can cause [35, 36].

Several studies have analyzed conventional and digital impression techniques, concluding that both procedures are clinically acceptable, and therefore, widely recommended. However, when studying the comparative accuracy of both techniques, results that can still be considered controversial begin to appear. Some authors suggest better results of the conventional technique over the digital technique, and others report better marginal adaptation of the digital technique than the conventional technique, thus confusing the professional who must make a scientifically supported clinical decision to provide high-quality prosthetic work with the greatest possible durability. A systematic review of the scientific literature could help evaluate the accuracy of these two techniques in a more comprehensive manner [37, 38].

For these reasons, this systematic review has been conducted to assess the compliance of the previous systematic reviews (SRs) on the accuracy (marginal adaptation and/or internal adaptation) of full-coverage fixed prostheses made with digital impressions versus conventional impressions with the requirements established by the scientific community in order to reveal the validity and reliability of each of these reviews and paint a clearer picture of clinical applicability when fabricating long-lasting fixed restorations.

2. MATERIALS AND METHODS

2.1. Protocol and Registration

A general protocol was developed based on the “preferred reporting items for systematic reviews and meta-analytical protocols (PRISMA-P) checklist” [39] and has been registered in the “International Platform of Registered Systematic Review and Meta-Analytical Protocols” (INPLASY). The registry is publicly available under the number INPLASY2021100024.

2.2. Eligibility Criteria

To be considered eligible, studies had to meet the following criteria:

- Systematic reviews with or without meta-analysis that have evaluated the accuracy (marginal adaptation and/or internal adaptation) of full-coverage fixed prostheses on natural teeth in clinical studies and on tooth replicas in *in vitro* studies.
- Systematic reviews with or without meta-analysis that have compared digital impressions made with an intraoral scanner versus conventional impressions taken with any type of impression material.
- Systematic reviews and/or meta-analyses of randomized clinical trials (RCTs) and comparative, prospective, nonrandomized, and *in vitro* clinical trials.

There were no time or language restrictions.

2.3. Exclusion Criteria

The studies excluded from this systematic review were the following:

- Literature reviews, case reports, and pilot studies
 - Studies that have evaluated seating in crowns on implants and partial restorations.
 - Studies whose authors did not respond to our requests for information.
 - Systematic reviews that did not meet the patient/population, intervention, comparison, and outcomes (PICO) framework parameters.

2.4. Sources of Information and Search Strategy

On July 17, 2020, an electronic search was conducted in three databases (Scopus, PubMed, and Web of Science). The gray literature was also searched through Google Scholar and the New York Academy of Medicine Gray Literature Report. The bibliography of the included studies was manually examined. The studies obtained were exported to the Mendeley bibliographic reference manager (Mendeley Desktop v 1.19.4.0), and duplicate studies were eliminated. The search strategy can be found in Appendix A. A search update was performed on September 22, 2021.

2.5. Study Selection

The selected studies were entered into Microsoft Excel, a software program for data analysis. Initially, two reviewers (M.A.C. and M.C.) independently selected the studies and read all their titles and abstracts to estimate if each article met the inclusion criteria. These two reviewers then read the full text of each remaining article. A third and fourth reviewer (J.A. and Y.A.) were consulted in case of disagreement. Finally, any studies that did not meet the inclusion criteria were excluded.

2.6. Data Collection

The information on the articles was collected using a table previously prepared by two reviewers (M.A.C. and M.C.) independently and combined. The data were compared, and discrepancies between authors were decided by a third and fourth reviewer (J.A. and Y.A.). The information extracted from the selected articles is shown in Table 1.

2.7. Assessment of Methodological Quality

The AMSTAR 2 tool, a measurement tool to assess systematic reviews, was used by two reviewers (M.A.C. and M.C.) to assess the methodological quality of the SRs included, independently and combined. AMSTAR 2 has 16 domains that can be answered with three possible answers: “yes”, “no”, or “partially yes” [40]. Seven of its domains are considered critical, since they can substantially affect the validity of a review and its conclusions. The general confidence (high, moderate, low, and critically low) of the studies was evaluated according to Shea *et al.* [40] as high: no or non-critical weaknesses; moderate: more than one non-critical weakness; low: a critical defect with or without non-critical or critical weaknesses; and critically low: more than one critical defect

with or without non-critical weaknesses. AMSTAR 2 does not generate an overall score, but the purpose of this tool is to identify high-quality systematic reviews.

2.8. Data Synthesis

The main results of each SR were categorized into the following topics: type of prosthetic restoration, marginal gap, internal gap, marginal discrepancy, marginal adaptation, and type of impression (Table 1). The data were visually presented as a traffic light plot where green represents the better marginal or internal adaptation, red represents poor marginal or internal adaptation, and yellow indicates no differences between the groups compared. The numerical data, the mean difference, and the relative risk can be found in Tables 2 and 3.

3. RESULTS

3.1. Review of Primary Study

From the search in the electronic databases and the gray literature, 131 references were obtained, of which 78 remained after eliminating duplicates. No articles from reference lists were added. Initially, the title and abstract of each chosen study

were assessed, and 22 articles were included for reading the full text.

The search was refreshed, in order to obtain recent information that can be included in the study but no new articles were found. Finally, six SRs were included for qualitative synthesis. The reasons for excluding SRs can be found in Appendix B. The complete process of the identification and selection of studies is presented in Fig. (1).

3.2. Assessment of Methodological Quality

Three systematic reviews [41 - 43] were considered to have low confidence, while the other three [36, 44, 45] were considered to have critically low confidence. The explanation of the design selection of the included studies, an exhaustive literature search strategy, and the mention of the sources of funding of the studies included in the SRs, corresponding to domains 3, 4, 10, and 16, respectively, were considered critical. None of the SRs met these criteria. One SR partially complied with domain 9 regarding the assessment of the risk of bias in the included studies [43]. More information on the evaluation of the methodological quality is provided in Fig. (1) and in Appendix C.

Table 1. Summary of the overall descriptive characteristics of the included systematic reviews (n = 6), part I.

Author (Year)/Ref	Population	Interventions and Comparators	Primary Studies	Mention of the following items: 1. PRISMA 2. PROSPERO 3. GRADE 4. Meta-analysis	Reported Review Limitations/Ref
Bandiaky <i>et al.</i> (2022) [41]	Fixed - supported prostheses	Intervention: digital scans Control: conventional impression techniques	Comparative studies, prospective: 2; randomized controlled clinical studies: 14	1. Yes 2. Yes 3. No 4. Yes	Few studies per parameter and few participants included in each study. Evidence level was low for the studies that were otherwise heterogeneous.. [41]
Chochlidakis <i>et al.</i> (2016) [36]	Fit of fixed dental restorations	Intervention: digital impression techniques Control: conventional impression techniques	Clinical studies: 2; in vitro studies: 9	1. Yes 2. No 3. No 4. Yes	Additional cost of purchasing an intraoral scanner and the learning curve for adjusting to the new technology [36]
Hasanzade <i>et al.</i> (2021) [42]	Fixed prostheses	Intervention: digital scanning and conventional fabrication and digital scanning and fabrication. Control: conventional impression and fabrication and conventional impression and digital fabrication	Clinical trials: 8; in vitro studies: 21	1. Yes 2. Yes 3. No 4. Yes	No mention
Hasanzade <i>et al.</i> (2019) [43]	Full-coverage restorations	Intervention: digital impression Control: conventional impression	Prospective clinical trials: 8; in vitro studies: 26	1. Yes 2. Yes 3. Yes 4. Yes	Uncontrolled factors may have had a direct influence on marginal and internal adaptation, including scanner type, finish line design, amount of spacer, fabrication technique, measurement of cemented or uncemented restorations, technical error during the laboratory stages, and adjustment of restorations. Subanalysis could not be performed due to the limited number of included studies. Only studies in English were included in the meta-analyses. [43]

(Table 1) cont....

Author (Year)/Ref	Population	Interventions and Comparators	Primary Studies	Mention of the following items: 1. PRISMA 2. PROSPERO 3. GRADE 4. Meta-analysis	Reported Review Limitations/Ref
Tabesh <i>et al.</i> (2021) [44]	Single-unit zirconia crowns	Intervention: digital scans Control: conventional impression	Prospective clinical trials: 8; in vitro studies: 11	1. Yes 2. Yes 3. No 4. Yes	Heterogeneity of the selected studies, including the different methods of tooth preparation, fabrication of restorations, and evaluation of marginal gaps. [44]
Tsirogiannis <i>et al.</i> (2016) [45]	Ceramic restorations	Intervention: digital impression Control: conventional impression	In vitro: 8; in vivo: 4	1. No 2. No 3. No 4. Yes	No mention

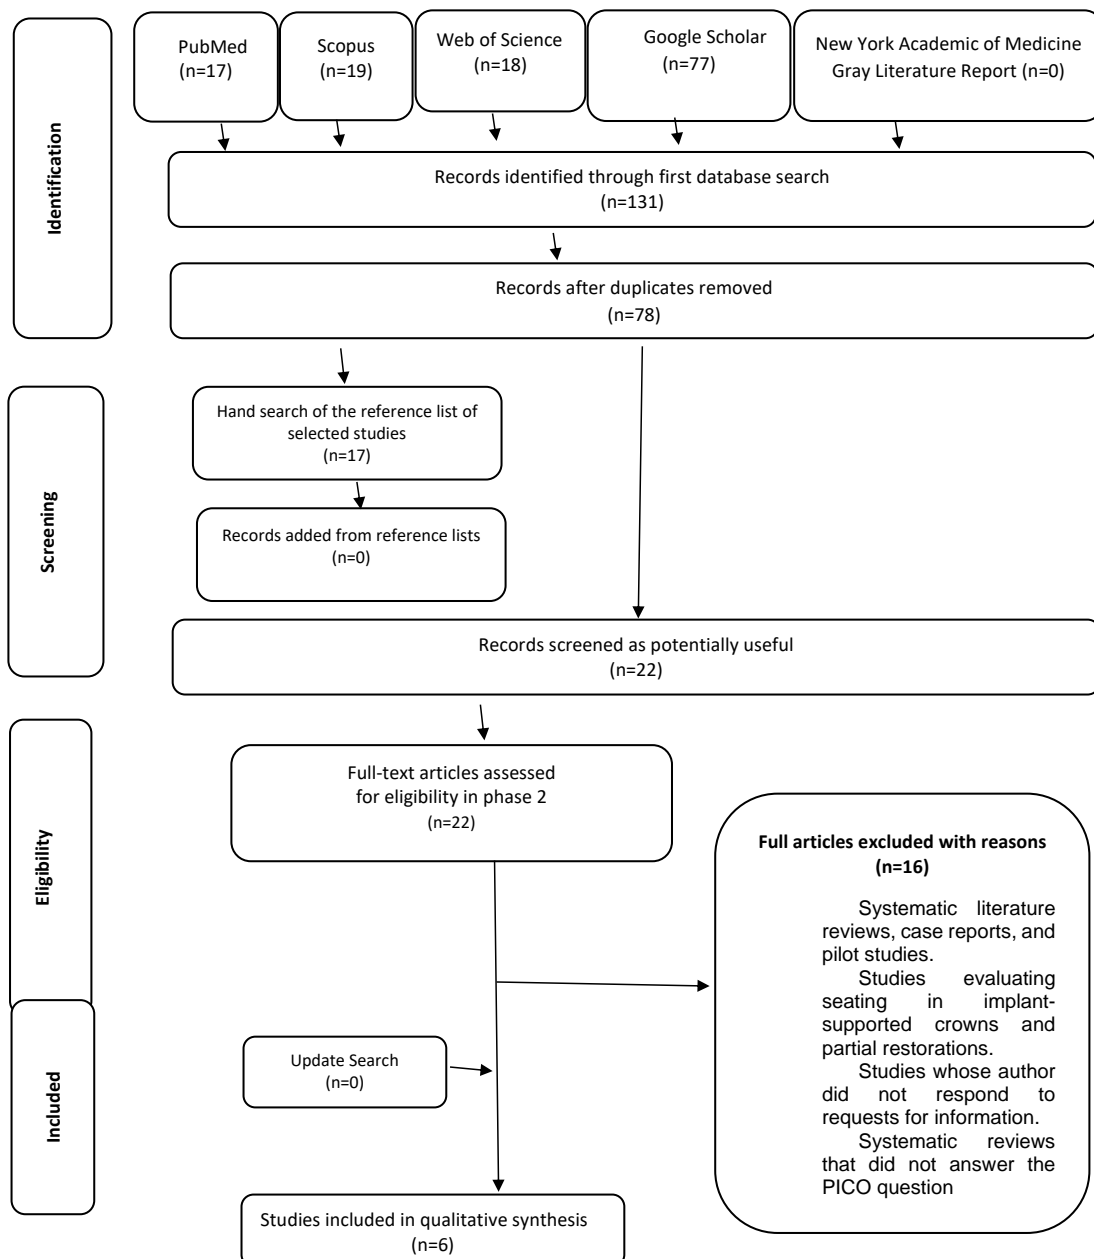


Fig. (1). Flow diagram of the literature search and selection criteria.

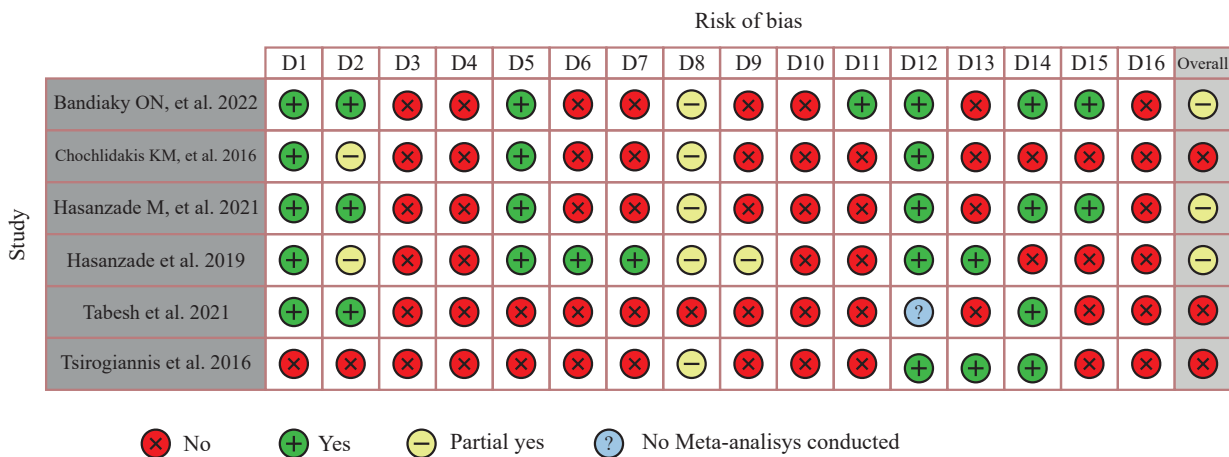


Fig. (2). Summary of the authors' judgments on each included SR, assessed by the critical appraisal tool for systematic reviews AMSTAR 2 and graphically represented as a traffic light plot, generated using robvis (a visualization tool). Green means “yes,” yellow “partially yes,” and red “no”. Blank cells represent the lack of meta-analysis on that question.

- D1 Did the research questions and inclusion criteria for the review include the components of PICO?
- D2 Did the report of the review contain an explicit statement that the review methods were established prior to the conduct of the review and did the report justify any significant deviations from the protocol?
- D3 Did the review authors explain their selection of the study designs for inclusion in the review?
- D4 Did the review authors use a comprehensive literature search strategy?
- D5 Did the review authors perform study selection in duplicate?
- D6 Did the review authors perform data extraction in duplicate?
- D7 Did the review authors provide a list of excluded studies and justify the exclusions?
- D8 Did the review authors describe the included studies in adequate detail?
- D9 Did the review authors use a satisfactory technique for assessing the risk of bias (RoB) in individual studies that were included in the review?
- D10 Did the review authors report on the sources of funding for the studies included in the review?
- D11 If meta-analysis was performed did the review authors use appropriate methods for statistical combination of results?
- D12 If meta-analysis was performed, did the review authors assess the potential impact of RoB in individual studies on the results of the meta-analysis or other evidence synthesis?
- D13 Did the review authors account for RoB in individual studies when interpreting/ discussing the results of the review?
- D14 Did the review authors provide a satisfactory explanation for, and discussion of, any heterogeneity observed in the results of the review?
- D15 If they performed quantitative synthesis did the review authors carry out an adequate investigation of publication bias (small study bias) and discuss its likely impact on the results of the review?
- D16 Did the review authors report any potential sources of conflict of interest, including any funding they received for conducting the review?

3.3. Synthesis of Results

The results of the literature synthesis are presented in Tables 2 and 3.

3.4. Marginal Fit/Marginal Gap/Marginal Adaptation/Marginal Discrepancy

The marginal discrepancy was defined by Holmes *et al.* as the vertical marginal discrepancy measured between the crown and the margins of the preparation under a 3D optical microscope [46].

The six SRs evaluated the adaptation or marginal fit [36, 41 - 45], and three SRs [36, 41, 45] showed no significant difference in the marginal adaptation of single-unit fixed prostheses between digital and conventional impressions. Three SRs [42 - 44] showed a better marginal adaptation with digital impressions (Table 2). The mean difference in marginal adaptation between digital and conventional impressions ranged from -0.59 (CI -0.93, -0.24) to -4.2 (CI: -33.0, 24.5) micrometers. One SR [45] reported a mean marginal adaptation of 27.2 micrometers (with a range of -5.3 to 59.7 micrometers) in *in vivo* studies and -4.2 micrometers (with a range of -33.0 to

24.5 micrometers) in *in vitro* studies. Chochlidakis *et al.* [36] performed a quantitative and qualitative analysis of *in vitro* studies and reported a mean marginal discrepancy of 0.24 (-0.32, 0.79) micrometers, but they only performed a qualitative analysis of *in vivo* studies due to the small number of included studies.

3.5. Internal Adaptation/Internal Gap

The internal discrepancy was defined by Holmes *et al.* as the perpendicular distance between the inner surface of the crown and the outer surface of the preparation under a 3D optical microscope [46]. Three studies measured internal adaptation [36, 42, 43]. Two studies [36, 43] reported no significant differences in internal adaptation in single-unit fixed prostheses fabricated with digital and conventional impressions, with a mean of 0.03 (-0.91, 0.96) micrometers and -0.17 (-0.53, - 0.20 micrometers) (Table 3). One study [42] reported an average of 0.32 micrometers (with a range of 0.08 to 0.56 micrometers), showing a better internal adaptation with digital impressions.

4. DISCUSSION













During the last decade, research has evaluated marginal and internal adaptation in single-unit fixed prostheses fabricated from a digital impression or a conventional impression, but the results have been contradictory, and the methods used to carry out these reviews have been unsatisfactory. Therefore, health professionals are basing their clinical decisions on unreliable studies. For this reason, the objective of this systematic review was to evaluate the methodological quality of the SRs currently published about the accuracy (marginal adaptation and/or internal adaptation) of full-coverage fixed prostheses made with digital impressions versus conventional impressions. AMSTAR 2 tool was applied to demonstrate the validity and reliability of each of these reviews.

When assessing the methodological quality of the SRs included in this study using the AMSTAR 2 tool, low reliability and low quality were found, especially in domains 3, 4, 10, and 16 of AMSTAR 2, since none of the SRs explained the selection of the study design, performed an exhaustive literature search, reported the sources of funding of the included studies, or reported the existence of possible sources of conflict of interest, including any funding received to conduct the review, considering these items in future SRs.

The studies included in the SRs showed high heterogeneity; some studies reported heterogeneity values above 75%, which is considered high. This can be explained by their use of different types of restorations [47] or laboratory fabrication techniques, types of scanner, amounts of spacer needed, preparation designs [48], and methods of measuring marginal adaptation (optical microscope [46, 49, 50], stereomicroscope, macroscope, or explorer). In addition, the majority of authors [51 - 56] used the silicone replica technique to measure the marginal fit of the crown before cementation, which is also a non-invasive practice with acceptable accuracy; however, this technique can lead to inaccuracies [43, 57].







Hasanzade *et al.* [43] performed an SR in 2019 that concluded single-unit fixed prostheses fabricated from a digital impression to show a better marginal adaptation than those fabricated from a conventional impression, while the internal adaptation did not show statistically significant differences between the two techniques. However, in 2020, Hasanzade *et al.* [42] performed another SR that found marginal adaptation and internal adaptation to be better with the digital approach than the conventional impression. This difference between the two studies can be because the first study did not specify the method used to make the crowns, while in the second study, fabrication was digital, and the scanners, design software, and dental milling machines were optimally combined and used to compensate for the error tolerance of each step [42, 43]

Table 2. Marginal gap/discrepancy marginal/marginal fit in the general results, graphically represented by colors, where green represents the treatment with the best results, red treatment with the worst results, and yellow that there are no differences between the compared groups.

Systematic Review	DI	CI	Reported Results	Studies for Comparison
Bandiaky <i>et al.</i> (2022), France, Journal of Prosthetic Dentistry [41]			Marginal fit: MD: -11.1 (C.I. = -32.5, 10.4), P > .05	Comparative studies, prospective (2), and randomized controlled clinical studies (14)
Chochlidakis <i>et al.</i> (2016), Journal of Prosthetic Dentistry [36]			Marginal discrepancy: MD: 0.24 (-0.32, 0.79), I2 = 82.64%, P < .001	Clinical studies (2) and <i>in vitro</i> studies (9)
Hasanzade <i>et al.</i> (2021), Iran, Journal of Prosthetic Dentistry [42]			Marginal gap: MD: 0.25 (0.09, 0.59), I2 = 66.5%, P = .006	Clinical trials (8) and <i>in vitro</i> studies (21)
Hasanzade <i>et al.</i> (2019), Iran, Journal of Evidence Based Dental Practice [43]			Marginal gap: MD: -0.59 (C.I. = -0.93, -0.24), I2 = 86%, P < 0.00001	Prospective clinical trials (8) and <i>in vitro</i> studies (26)
Tabesh <i>et al.</i> (2021), Iran, Journal of Prosthetic Dentistry [44]			Marginal gap: MD: -0.89 (-1.24, -0.54), I2 = 78.2%, P < .001	Prospective clinical trials (8) and <i>in vitro</i> studies (11)
Tsirogianis <i>et al.</i> (2016), Germany, Journal of Prosthetic Dentistry [45]			Discrepancy marginal <i>in vivo</i> : adjusted MD: 27.2 (C.I. = -5.3, 59.7), P = .084	4 <i>in vivo</i> studies
			Discrepancy marginal <i>in vitro</i> : adjusted MD: -4.2 (C.I. = -33.0, 24.5), P = .763	8 <i>in vitro</i> studies

Abbs DI, digital printing; CI, conventional printing; MD, mean difference; CI, confidence interval.

Table 3. Internal gap/internal adaptation in the general results graphically represented by colors, where green represents the treatment with the best results, red treatment with worse results, and amber indicates that there are no differences between compared groups.

Systematic review	DI	CI	Reported results	Studies for comparison
Bandiaky <i>et al.</i> (2022), France, Journal of Prosthetic Dentistry [41]			Internal gap: MD: 0.03 (-0.91, 0.96), I2 = 92.22%, P < .0001	Comparative studies, prospective (2) and randomized controlled clinical studies (14)
Hasanzade <i>et al.</i> (2021), Iran, Journal of Prosthetic Dentistry [42]			Internal adaptation: MD: 0.32 (C.I. = 0.08, 0.56), I2 = 0.0%, P = .457	Clinical trials (8) and <i>in vitro</i> studies (21)
Hasanzade <i>et al.</i> (2019), Iran, Journal of Evidence Based Dental Practice [43]			Internal gap: MD: -0.17 (C.I. = - 0.53, -0.20), I2 = 86%, P < 0.00001	Prospective clinical trials (8) and <i>in vitro</i> studies (26)

DI, digital printing; CI, conventional printing; MD, mean difference; CI, confidence interval.

Tsirogiannis *et al.* [45] found no significant difference in the marginal discrepancy of single-unit ceramic restorations fabricated after digital and conventional impressions, either *in vivo* or *in vitro* studies. However, in the SR performed by Hasanzade *et al.* [43], they determined no significant differences between the digital and conventional groups in *in vivo* studies, but in *in vitro* studies, digital impressions resulted in better marginal adaptation. Mai *et al.* [58], in their SR, found the marginal adaptation values measured by digital methods to be nominally higher but not significantly different from those measured by conventional methods in *in vitro* studies. Morsy *et al.* [59] found digital scanning to provide a significantly better marginal fit than conventional impression for fabricating fixed partial dentures of up to four units, either in monolithic form or structures and in any region of the arch.

Nagarkar *et al.* [51] indicated that, in marginal and internal adaptation, there were no significant differences between the impression techniques.

The clinical use of digital impressions is constantly increasing due to their various advantages. This technology eliminates the selection of trays and impression materials and facilitates electronic transfer, the storage of digital files, and in-office milling of final restorations [16]. The limitations of digital impressions include the additional costs related to the purchase of an intraoral scanner, the need to participate in courses and workshops, and the need to constantly update with advancing technology.

When performing this systematic review, it was observed that despite many SRs, there was an urgent need to establish a standardized protocol to improve the quality of their reporting using assessment tools, such as AMSTAR 2. In addition, it is suggested to improve the inclusion and exclusion criteria of future research, with the aim of increasing the methodological homogeneity of primary studies. Likewise, new primary studies (RCTs) should be done with high methodological rigor to yield more reliable results and high-quality SRs.

Future studies should have a standardized protocol regarding the type of restoration, preparation design, conventional impression material, laboratory fabrication technique, amount of spacer needed, type of scanner, and methods used to measure the marginal adaptation so that they can all compare marginal and internal fit in a similar way.

CONCLUSION

From the limitations of the SRs included in the present study, the following conclusions can be drawn.

- The methodological quality of published SRs is poor according to the AMSTAR 2 tool, making for low and critically low confidence. In addition, some reviews used the original MINORS scale to evaluate the methodological quality of their included studies, which has not been validated in terms of content or scoring.
- The studies included in the SRs showed high heterogeneity; the number of clinical studies in the SRs was small, which made it difficult for some SRs to perform a quantitative analysis of them, and some SRs included only studies in English.
- Half of the systematic reviews showed a better marginal adaptation with digital impressions, while the other half showed no significant differences between conventional and digital impressions.
- Internal adaptation was better with digital impressions in one SR, while two SRs did not show statistically significant differences between conventional and digital impressions.

LIST OF ABBREVIATIONS

- CAD/CAM** = Computer-aided design and manufacturing
- SRs** = Systematic reviews
- PRISMA-P** = Preferred reporting items for systematic reviews and meta-analytical protocols
- INPLASY** = International Platform of Registered Systematic Review and Meta-Analytical Protocols
- RCTs** = Randomized Clinical Trials
- PICO** = Patient/Population, Intervention, Comparison, Outcomes
- GRADE** = Grading of Recommendations Assessment, Development, and Evaluation
- AMSTAR 2** = A Measurement Tool to Assess Systematic Reviews
- DI** = Digital Printing
- CI** = Conventional Printing

MD = Mean Difference

CI = Confidence Interval

CONSENT FOR PUBLICATION

Not applicable.

STANDARDS OF REPORTING

PRISMA guidelines were followed.

AVAILABILITY OF DATA AND MATERIALS

The data supporting the findings of the article is available in the Zenodo at <https://zenodo.org/record/7746657#.ZBSxxnbMLb0>.

FUNDING

None.

CONFLICT OF INTEREST

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

ACKNOWLEDGEMENTS

The authors thank the Faculty of Dentistry of the University of Cuenca, Ecuador.

SUPPLEMENTARY MATERIALS

PRISMA checklist is available as supplementary material on the publisher's website along with the published article.

APPENDIX

Appendix A.SEARCH STRATEGY		
P	-	-
PUBMED	("posterior fixed" OR "dental porcelain"[Mesh] OR "single-unit" OR "crowns"[Mesh] OR "full-coverage restorations"OR "fixed prosthodontics" OR "fixed dental prostheses")	36.99 5
WOS	TÍTULO: ("posterior fixed" OR "dental porcelain"OR "singleunit" OR "crowns"OR "full-coverage restorations"OR "fixed prosthodontics" OR "fixed dental prostheses")	6.440
SCOPUS	TITLE-ABS-KEY ("posterior fixed" OR "dental porcelain" OR "singleunit" OR "crowns" OR "full-coverage restorations" OR "fixed prosthodontics" OR "fixed dental prostheses")	164,6 35
GOOGLE SCHOLAR	("posterior fixed" OR "dental porcelain" OR "single-unit" OR "crowns" OR "full-coverage restorations"OR "fixed prosthodontics" OR "fixed dental prostheses")	939.0 00
NEW YORK ACADEMIC OF MEDICIN	-	-
GRAY LITERATUR E REPORT.	("posterior fixed" OR "dental porcelain"OR "single-unit" OR "crowns"OR "full-coverage restorations"OR "fixed prosthodontics" OR "fixed dental prostheses")	0
I	-	-
PUBMED	("digital" OR "digital scans" OR "digital impressions")	148
WOS	TÍTULO: ("digital" OR "digital scans" OR "digital impressions")	204.3 77
SCOPUS	TITLE-ABS-KEY ("digital" OR "digital scans" OR "digital impressions")	1 ,186, 959
GOOGLE SCHOLAR	("digital" OR "digital scans" OR "digital impressions")	7.160. 000
C	-	-
PUBMED	("conventional impressions" OR "manual impressions" OR "conventional")	501
WOS	TÍTULO: ("conventional impressions" OR "manual impressions" OR "conventional")	75.25 9
SCOPUS	TITLE-ABS-KEY ("conventional impressions" OR "manual impressions" OR "conventional")	1 ,706, 645
GOOGLE SCHOLAR	("conventional impressions" OR "manual impressions" OR "conventional")	5.790. 000
O	-	-
PUBMED	("accuracy" OR "adaptations" OR "dimensional accuracy" OR "marginal fit" OR "internal fit" OR "adjustment")	650.3 26
WOS	TÍTULO: ("accuracy" OR "adaptations" OR "dimensional accuracy" OR "marginal fit" OR "internal fit" OR "adjustment")	158.2 62
SCOPUS	TITLE-ABS-KEY ("accuracy" OR "adaptations" OR "dimensional accuracy" OR "marginal fit" OR "internal fit" OR "adjustment")	3 ,108, 658
GOOGLE SCHOLAR	("accuracy" OR "adaptations" OR "dimensional accuracy" OR "marginal fit" OR "internal fit" OR "adjustment")	5.970. 000
S	-	-
PUBMED	("systematic review and meta-analysis" OR "systematic review" OR "meta- analysis")	306.0 94
WOS	TÍTULO: ("systematic review and meta-analysis" OR "systematic review" OR "meta- analysis")	232.0 01
SCOPUS	TITLE-ABS-KEY ("systematic review and meta-analysis" OR "systematic review" OR "meta- analysis")	457,2 26
GOOGLE SCHOLAR	("systematic review and meta-analysis" OR "systematic review" OR "meta- analysis")	17.80 0

Appendix A. SEARCH STRATEGY		
P		
	-	-
	-	-
PUBMED	("posterior fixed" OR "dental porcelain"[Mesh] OR "single-unit" OR "crowns"[Mesh] OR "full-coverage restorations"OR "fixed prosthodontics" OR "fixed dental prostheses") AND ("digital" OR "digital scans" OR "digital impressions") AND ("conventional impressions" OR "manual impressions" OR "conventional") AND ("accuracy" OR "adaptations" OR "dimensional accuracy" OR "marginal fit" OR "internal fit" OR "adjustment") AND ("systematic review and meta-analysis" OR "systematic review" OR "meta- analysis")	17
WOS	TEMA: ("posterior fixed" OR "dental porcelain"OR "singleunit" OR "crowns"OR "full-coverage restorations"OR "fixed prosthodontics" OR "fixed dental prostheses") AND TEMA: ("digital" OR "digital scans" OR "digital impressions") AND TEMA: ("conventional impressions" OR "conventional") AND TEMA: ("accuracy" OR "adaptation s" OR "dimensional accuracy" OR "marginal fit" OR "internal fit" OR "adjustment") AND TEMA: ("systematic review and metaanalysis" OR "systematic review" OR "meta- analysis")	19
SCOPUS	(TITLE-ABS-KEY ("posterior fixed" OR "dental porcelain" OR "singleunit" OR "crowns" OR "full-coverage restorations" OR "fixed prosthodontics" OR "fixed dental prostheses") AND TITLE-ABS-KEY ("digital" OR "digital scans" OR "digital impressions") AND TITLE-ABS-KEY ("conventional impressions" OR "manual impressions" OR "conventional") AND TITLE-ABS-KEY ("accuracy" OR "adaptations" OR "dimensional accuracy" OR "marginal fit" OR "internal fit" OR "adjustment") AND TITLE-ABS-KEY ("systematic review and metaanalysis" OR "systematic review" OR "meta- analysis")	18
GOOGLE SCHOLAR	in title: ("crowns") AND ("digital impressions") AND ("conventional impressions") AND ("accuracy") AND ("systematic review and meta-analysis")	77
NEW YORK ACADEMIC OF MEDICIN GRAY LITERATUR E REPORT.	("crowns") AND ("digital impressions") AND ("conventional impressions") AND ("accuracy") AND ("systematic review and meta- analysis")	0

Appendix B. Articles excluded from the study	
Study	Reason for exclusion
[Ahlholm P et al. 2018]	2
[Ahmed WM, et al. 2020]	1
[Al-Haj Husain N, et al. 2020]	2
[Arcuri L, et al. 2019]	3
[Carvalho T, et al. 2018]	1
[Chandran S, et al. 2019]	2
[Cicciù M, et al. 2020]	4
[Gallardo Y, et al. 2018]	4
[Giachetti L, et al. 2020]	2
[Kumar H, et al. 2020]	4
[Kyoung-Rok Kim, et al. 2018]	4
[Mai H, et al. 2020]	4
[Nagarkar S, et al. 2018]	4
[Papadiochou S, et al. 2017]	2
[Pecciarini M, et al. 2019]	2
[Svanborg P, et al. 2020]	2
1	Systematic reviews of the literature, case reports, pilot studies
2	Studies evaluating seating in implant crowns and partial restorations
3	Studies without response from the author to the information query requested
4	Systematic reviews that do not meet the PICO question

Appendix C. AMSTAR 2 assessment criteria and domains																		
Study	Q 1	Q 2	Q 3	Q 4	Q 5	Q 6	Q 7	Q 8	Q 9	Q 10	Q 11	Q 12	Q 13	Q 14	Q 15	Q 16	Overall confidence	
Bandiaky ON, et al. 2020	Y	Y	N	N	Y	N	N	P	Y	N	Y	Y	N	Y	Y	N	Low	
Chochlidakis KM, et al. 2016	Y	P	Y	N	Y	N	N	P	Y	N	N	Y	N	N	N	N	Critically low	
Hasanzade M, et al. 2020	Y	Y	N	N	Y	N	N	P	Y	N	N	Y	N	Y	Y	N	Low	
Hasanzade et al. 2019	Y	P	Y	N	Y	Y	Y	P	Y	P	Y	N	Y	Y	N	N	Low	
Tabesh et al. 2020	Y	Y	N	N	N	N	N	N	N	N	N	N	M	A	N	Y	N	Critically low
Tsirogiannis et al. 2016	N	N	N	N	N	N	N	P	Y	N	N	N	Y	Y	Y	N	N	Critically low
Y	YES																	
N	NO																	
PY	PARTIAL YES																	
NMA	NO META- ANALISIS																	

REFERENCES

[1] Moörmann WH. The evolution of the CEREC system. J Am Dent Assoc 2006; 137(Suppl.): 7S-13S. [http://dx.doi.org/10.14219/jada.archive.2006.0398] [PMID: 16950932]

[2] Garcia-Gil I, Perez de la Calle C, Lopez-Suarez C, Pontevedra P, Suarez MJ. Comparative analysis of trueness between conventional and digital impression in dental-supported fixed dental prosthesis with vertical preparation. J Clin Exp Dent 2020; 12(9): e896-901. [http://dx.doi.org/10.4317/jced.56967] [PMID: 32994882]

[3] Zeltner M, Sailer I, Mühlemann S, Özcan M, Hämmerle CHF, Benic GI. Randomized controlled within-subject evaluation of digital and conventional workflows for the fabrication of lithium disilicate single crowns. Part III: marginal and internal fit. J Prosthet Dent 2017; 117(3): 354-62. [http://dx.doi.org/10.1016/j.prosdent.2016.04.028] [PMID: 27677220]

[4] Ahlholm P, Sipilä K, Vallittu P, Jakonen M, Kotiranta U. Digital versus conventional impressions in fixed prosthodontics: a review. J Prosthodont 2018; 27(1): 35-41. [http://dx.doi.org/10.1111/jopr.12527] [PMID: 27483210]

[5] Syrek A, Reich G, Ranftl D, Klein C, Cerny B, Brodessa J. Clinical evaluation of all-ceramic crowns fabricated from intraoral digital impressions based on the principle of active wavefront sampling. J Dent 2010; 38(7): 553-9. [http://dx.doi.org/10.1016/j.jdent.2010.03.015] [PMID: 20381576]

[6] Seelbach P, Brueckel C, Wöstmann B. Accuracy of digital and conventional impression techniques and workflow. Clin Oral Investig 2013; 17(7): 1759-64. [http://dx.doi.org/10.1007/s00784-012-0864-4] [PMID: 23086333]

[7] Fasbinder DJ. Digital dentistry: innovation for restorative treatment. Compend Contin Educ Dent 2010; 31(Spec No 4): 2-11. [PMID: 21049823]

[8] Wiersema EJ, Kreulen CM, Creugers NHJ. [The conventional and the digital impression method for single-unit and multi-unit fixed dental prostheses]. Ned Tijdschr Tandheelkd 2013; 120(7-8): 401-10. [http://dx.doi.org/10.5177/mtvt.2013.07.08.13170] [PMID: 23923443]

[9] Svanborg P, Skjervén H, Carlsson P, Eliasson A, Karlsson S, Örtorp A. Marginal and internal fit of cobalt-chromium fixed dental prostheses generated from digital and conventional impressions. Int J Dent 2014; 2014: 1-9. [http://dx.doi.org/10.1155/2014/534382] [PMID: 24723954]

[10] Haddadi Y, Bahrami G, Isidor F. Accuracy of intra-oral scans compared to conventional impression *in vitro*. Prim Dent J 2019; 8(3): 34-9. [http://dx.doi.org/10.1308/205016819827601491] [PMID: 31666171]

[11] Hans JS. Dental impressions: Metal rim lock trays. Br Dent J 2016; 220(3): 89-90. [http://dx.doi.org/10.1038/sj.bdj.2016.69] [PMID: 26868775]

[12] Miyazaki T, Hotta Y, Kunii J, Kuriyama S, Tamaki Y. A review of dental CAD/CAM: current status and future perspectives from 20 years of experience. Dent Mater J 2009; 28(1): 44-56. [http://dx.doi.org/10.4012/dmj.28.44] [PMID: 19280967]

[13] Christensen GJ. Impressions are changing: deciding on conventional, digital or digital plus in-office milling. J Am Dent Assoc 2009; 140(10): 1301-4. [http://dx.doi.org/10.14219/jada.archive.2009.0054] [PMID: 19797561]

[14] Beuer F, Schweiger J, Edelhoff D. Digital dentistry: an overview of recent developments for CAD/CAM generated restorations. Br Dent J 2008; 204(9): 505-11. [http://dx.doi.org/10.1038/sj.bdj.2008.350] [PMID: 18469768]

[15] Haddadi Y, Bahrami G, Isidor F. Evaluation of operating time and patient perception using conventional impression taking and intraoral scanning for crown manufacture: a split-mouth, randomized clinical study. Int J Prosthodont 2018; 31(1): 55-9. [http://dx.doi.org/10.11607/ijp.5405] [PMID: 29145527]

[16] Lee SJ, Gallucci GO. Digital vs. conventional implant impressions: efficiency outcomes. Clin Oral Implants Res 2013; 24(1): 111-5. [http://dx.doi.org/10.1111/j.1600-0501.2012.02430.x] [PMID: 22353208]

[17] Galhano GÁP, Pellizzer EP, Mazaro JVQ. Optical impression systems for CAD-CAM restorations. J Craniofac Surg 2012; 23(6): e575-9. [http://dx.doi.org/10.1097/SCS.0b013e31826b8043] [PMID: 23172483]

[18] Davidowitz G, Kotick PG. The use of CAD/CAM in dentistry. Dent Clin North Am 2011; 55(3): 559-70. [http://dx.doi.org/10.1016/j.cden.2011.02.011] [PMID: 21726690]

[19] Pradies G, Zarauz C, Valverde A, Ferreira A, Martínez-Rus F. Clinical evaluation comparing the fit of all-ceramic crowns obtained from silicone and digital intraoral impressions based on wavefront sampling technology. J Dent 2015; 43(2): 201-8. [http://dx.doi.org/10.1016/j.jdent.2014.12.007] [PMID: 25527248]

[20] Conrad HJ, Seong WJ, Pesun IJ. Current ceramic materials and systems with clinical recommendations: A systematic review. J Prosthet Dent 2007; 98(5): 389-404. [http://dx.doi.org/10.1016/S0022-3913(07)60124-3] [PMID: 18021828]

[21] van Noort R. The future of dental devices is digital. Dent Mater 2012; 28(1): 3-12. [http://dx.doi.org/10.1016/j.dental.2011.10.014] [PMID: 22119539]

[22] Almeida e Silva JS, Erdelt K, Edelhoff D, et al. Marginal and internal fit of four-unit zirconia fixed dental prostheses based on digital and conventional impression techniques. Clin Oral Investig 2014; 18(2): 515-23. [http://dx.doi.org/10.1007/s00784-013-0987-2] [PMID: 23716064]

[23] Beuer F, Naumann M, Gernet W, Sorensen JA. Precision of fit: zirconia three-unit fixed dental prostheses. Clin Oral Investig 2009; 13(3): 343-9. [http://dx.doi.org/10.1007/s00784-008-0224-6] [PMID: 18769946]

[24] Kumar H, Kumar T, Hemchand S, Suneelkumar C, Subha A. Accuracy of marginal adaptation of posterior fixed dental prosthesis made from digital impression technique: A systematic review. J Indian Prosthodont Soc 2020; 20(2): 123-30. [http://dx.doi.org/10.4103/jips.jips_382_19] [PMID: 32655216]

[25] Abdel-Azim T, Rogers K, Elathamna E, Zandinejad A, Metz M, Morton D. Comparison of the marginal fit of lithium disilicate crowns fabricated with CAD/CAM technology by using conventional impressions and two intraoral digital scanners. J Prosthet Dent 2015; 114(4): 554-9. [http://dx.doi.org/10.1016/j.prosdent.2015.04.001] [PMID: 26100929]

[26] Ahmed WM, Shariati B, Gazzaz AZ, Sayed ME, Carvalho RM. Comparison of marginal fit of cemented zirconia copings manufactured after digital impression with lava™ C.O.S and conventional impression technique. BMC Oral Health 2020; 6(6): 700-16.

- [27] Berrendero S, Salido MP, Valverde A, Ferreiroa A, Pradies G. Influence of conventional and digital intraoral impressions on the fit of CAD/CAM-fabricated all-ceramic crowns. *Clin Oral Investig* 2016; 20(9): 2403-10. [http://dx.doi.org/10.1007/s00784-016-1714-6] [PMID: 26800669]
- [28] Sailer I, Fehér A, Filser F, Gauckler LJ, Lüthy H, Hammerle CHF. Five-year clinical results of zirconia frameworks for posterior fixed partial dentures. *Int J Prosthodont* 2007; 20(4): 383-8. [PMID: 17695869]
- [29] Knoernschild KL, Campbell SD. Periodontal tissue responses after insertion of artificial crowns and fixed partial dentures. *J Prosthet Dent* 2000; 84(5): 492-8. [http://dx.doi.org/10.1067/mpr.2000.110262] [PMID: 11105004]
- [30] Sakornwimon N, Leevaloj C. Clinical marginal fit of zirconia crowns and patients' preferences for impression techniques using intraoral digital scanner versus polyvinyl siloxane material. *J Prosthet Dent* 2017; 118(3): 386-91. [http://dx.doi.org/10.1016/j.prosdent.2016.10.019] [PMID: 28222872]
- [31] Anadioti E, Aquilino SA, Gratton DG, et al. 3D and 2D marginal fit of pressed and CAD/CAM lithium disilicate crowns made from digital and conventional impressions. *J Prosthodont* 2014; 23(8): 610-7. [http://dx.doi.org/10.1111/jopr.12180] [PMID: 24995593]
- [32] Bader JD, Rozier RG, McFall WT Jr, Ramsey DL. Effect of crown margins on periodontal conditions in regularly attending patients. *J Prosthet Dent* 1991; 65(1): 75-9. [http://dx.doi.org/10.1016/0022-3913(91)90053-Y] [PMID: 2033551]
- [33] Jahn KR, Baum W, Zuhrt R. [Secondary caries frequency under complete crowns in relation to the material and design of the crown as well as the crown margin finish]. *Stomatol DDR* 1985; 35(11): 665-70. [PMID: 3915157]
- [34] Zoellner A, Brägger U, Fellmann V, Gaengler P. Correlation between clinical scoring of secondary caries at crown margins and histologically assessed extent of the lesions. *Int J Prosthodont* 2000; 13(6): 453-9. [PMID: 11203669]
- [35] Tabesh M, Alikhasi M, Siadat H. A Comparison of implant impression precision: Different materials and techniques. *J Clin Exp Dent* 2018; 10(2): e151-7. [PMID: 29670733]
- [36] Chochlidakis KM, Papispyridakos P, Geminiani A, Chen CJ, Feng JJ, Ercoli C. Digital versus conventional impressions for fixed prosthodontics: A systematic review and meta-analysis. *J Prosthet Dent* 2016; 116(2): 184-190.e12. [http://dx.doi.org/10.1016/j.prosdent.2015.12.017] [PMID: 26946916]
- [37] Euán R, Figueras-Álvarez O, Cabratosa-Termes J, Oliver-Parra R. Marginal adaptation of zirconium dioxide copings: Influence of the CAD/CAM system and the finish line design. *J Prosthet Dent* 2014; 112(2): 155-62. [http://dx.doi.org/10.1016/j.prosdent.2013.10.012] [PMID: 24445027]
- [38] Cetik S, Bahrami B, Fossoyeux I, Atash R. Adaptation of zirconia crowns created by conventional versus optical impression: *in vitro* study. *J Adv Prosthodont* 2017; 9(3): 208-16. [http://dx.doi.org/10.4047/jap.2017.9.3.208] [PMID: 28680553]
- [39] Shamseer L, Moher D, Clarke M, et al. Preferred reporting items for systematic review and meta-analysis protocols (PRISMA-P) 2015: elaboration and explanation. *BMJ* 2015; 350(1): g7647. [http://dx.doi.org/10.1136/bmj.i4086] [PMID: 25975279]
- [40] Shea BJ, Reeves BC, Wells G, et al. AMSTAR 2: a critical appraisal tool for systematic reviews that include randomised or non-randomised studies of healthcare interventions, or both. *BMJ* 2017; 358: j4008. [http://dx.doi.org/10.1136/bmj.j4008] [PMID: 28935701]
- [41] Bandiaky ON, Le Bars P, Gaudin A, et al. Comparative assessment of complete-coverage, fixed tooth-supported prostheses fabricated from digital scans or conventional impressions: A systematic review and meta-analysis. *J Prosthet Dent* 2022; 127(1): 71-9. [http://dx.doi.org/10.1016/j.prosdent.2020.09.017] [PMID: 33143901]
- [42] Hasanzade M, Aminikhah M, Afrashtehfar KI, Alikhasi M. Marginal and internal adaptation of single crowns and fixed dental prostheses by using digital and conventional workflows: A systematic review and meta-analysis. *J Prosthet Dent* 2021; 126(3): 360-8. [http://dx.doi.org/10.1016/j.prosdent.2020.07.007] [PMID: 32928518]
- [43] Hasanzade M, Shirani M, Afrashtehfar KI, Naseri P, Alikhasi M. *In vivo* and *in vitro* comparison of internal and marginal fit of digital and conventional impressions for full-coverage fixed restorations: a systematic review and meta-analysis. *J Evid Based Dent Pract* 2019; 19(3): 236-54. [http://dx.doi.org/10.1016/j.jebdp.2019.04.003] [PMID: 31732100]
- [44] Tabesh M, Nejatidanesh F, Savabi G, Davoudi A, Savabi O, Mirmohammadi H. Marginal adaptation of zirconia complete-coverage fixed dental restorations made from digital scans or conventional impressions: A systematic review and meta-analysis. *J Prosthet Dent* 2021; 125(4): 603-10. [http://dx.doi.org/10.1016/j.prosdent.2020.01.035] [PMID: 32284188]
- [45] Tsirogiannis P, Reissmann DR, Heydecke G. Evaluation of the marginal fit of single-unit, complete-coverage ceramic restorations fabricated after digital and conventional impressions: A systematic review and meta-analysis. *J Prosthet Dent* 2016; 116(3): 328-335.e2. [http://dx.doi.org/10.1016/j.prosdent.2016.01.028] [PMID: 27061627]
- [46] Souza ROA, Özcan M, Pavanelli CA, et al. Marginal and internal discrepancies related to margin design of ceramic crowns fabricated by a CAD/CAM system. *J Prosthodont* 2012; 21(2): 94-100. [http://dx.doi.org/10.1111/j.1532-849X.2011.00793.x] [PMID: 22050205]
- [47] Papadiochou S, Pissiotis AL. Marginal adaptation and CAD-CAM technology: A systematic review of restorative material and fabrication techniques. *J Prosthet Dent* 2018; 119(4): 545-51. [http://dx.doi.org/10.1016/j.prosdent.2017.07.001] [PMID: 28967399]
- [48] Cho L, Choi J, Jin Yi Y, Jin Park C. Effect of finish line variants on marginal accuracy and fracture strength of ceramic optimized polymer/fiber-reinforced composite crowns. *J Prosthet Dent* 2004; 91(6): 554-60. [http://dx.doi.org/10.1016/j.prosdent.2004.03.004] [PMID: 15211298]
- [49] Miwa A, Kori H, Tsukiyama Y, Kuwatsuru R, Matsushita Y, Koyano K. Fit of e.max crowns fabricated using conventional and CAD/CAM technology: a comparative study. *Int J Prosthodont* 2016; 29(6): 602-7. [http://dx.doi.org/10.11607/jip.4865] [PMID: 27824983]
- [50] Shembesh M, Ali A, Finkelman M, Weber HP, Zandparsa R. An *in vitro* comparison of the marginal adaptation accuracy of CAD/CAM restorations using different impression systems. *J Prosthodont* 2017; 26(7): 581-6. [http://dx.doi.org/10.1111/jopr.12446] [PMID: 26855068]
- [51] Nagarkar SR, Perdigão J, Seong WJ, Theis-Mahon N. Digital versus conventional impressions for full-coverage restorations. *J Am Dent Assoc* 2018; 149(2): 139-147.e1. [http://dx.doi.org/10.1016/j.adaj.2017.10.001] [PMID: 29389337]
- [52] Ahrberg D, Lauer HC, Ahrberg M, Weigl P. Evaluation of fit and efficiency of CAD/CAM fabricated all-ceramic restorations based on direct and indirect digitalization: a double-blinded, randomized clinical trial. *Clin Oral Investig* 2016; 20(2): 291-300. [http://dx.doi.org/10.1007/s00784-015-1504-6] [PMID: 26070435]
- [53] Haddadi Y, Bahrami G, Isidor F. Accuracy of crowns based on digital intraoral scanning compared to conventional impression—a split-mouth randomised clinical study. *Clin Oral Investig* 2019; 23(11): 4043-50. [http://dx.doi.org/10.1007/s00784-019-02840-0] [PMID: 30796587]
- [54] Malaguti G, Rossi R, Marziali B, et al. *In vitro* evaluation of prosthodontic impression on natural dentition: A comparison between traditional and digital techniques. *Oral Implantol* 2016; 9(S1): 21-7. [http://dx.doi.org/10.11138/orl/2016.9.S.021] [PMID: 28280529]
- [55] Benic GI, Sailer I, Zeltner M, Gütermann JN, Özcan M, Mühlemann S. Randomized controlled clinical trial of digital and conventional workflows for the fabrication of zirconia-ceramic fixed partial dentures. Part III: Marginal and internal fit. *J Prosthet Dent* 2019; 121(3): 426-31. [http://dx.doi.org/10.1016/j.prosdent.2018.05.014] [PMID: 30396708]
- [56] Laurent M, Scheer P, Dejou J, Laborde G. Clinical evaluation of the marginal fit of cast crowns - validation of the silicone replica method. *J Oral Rehabil* 2008; 35(2): 116-22. [http://dx.doi.org/10.1111/j.1365-2842.2003.01203.x] [PMID: 18197844]
- [57] Nawafleh NA, Mack F, Evans J, Mackay J, Hatamleh MM. Accuracy and reliability of methods to measure marginal adaptation of crowns and FDPs: A literature review. *J Prosthodont* 2013; 22(5): 419-28. [http://dx.doi.org/10.1111/jopr.12006] [PMID: 23289599]
- [58] Mai HY, Lee WK, Kwon TG, Lee DH. Reliability of digital measurement methods on the marginal fit of fixed prostheses: A systematic review and meta-analysis of *in vitro* studies. *J Prosthet Dent* 2020; 124(3): 350.e1-350.e11. [http://dx.doi.org/10.1016/j.prosdent.2020.04.011] [PMID: 32665119]
- [59] Morsy N, El Kateb M, Azer A, Fathalla S. Fit of zirconia fixed partial dentures fabricated from conventional impressions and digital scans: a systematic review and meta-analysis. *J Prosthet Dent* 2021; S0022-3913(21): 00496. [http://dx.doi.org/10.1016/j.prosdent.2021.08.025] [PMID: 34696907]