

Mechanical Integrity of All-on-Four Dental Implant Systems: Finite Element Simulation of Material Properties of Zirconia, Titanium, and PEEK



Che-Lun Chang^{1,#}, Riya Karmakar^{2,#}, Arvind Mukundan², Shu-Hao Lu³, Ubol Choomjinda⁴, Meei-Maan Chen⁵, Yi-Ling Chen^{6,*} and Hsiang-Chen Wang^{2,7,8,*}

¹Department of Oral-Maxillofacial Surgery, Taitung MacKay Memorial Hospital, No. 1, Ln. 303, Changsha St., Taitung City, Taitung County 950408, Taiwan

²Department of Mechanical Engineering, National Chung Cheng University, 168, University Rd., Min Hsiung, Chia Yi 62102, Taiwan

³Topology Medical Consultant Co., 12F., No. 812, Xincheng Rd., Qianzhen Dist., Kaohsiung City 80284, Taiwan

⁴School of Nursing, Shinawatra University, 99 Moo 10, Bangtoey, Samkhok, Pathum Thani 12160, Thailand

⁵Center for Innovative Research on Aging Society (CIRAS), National Chung Cheng University, 168, University Rd., Min Hsiung, Chia Yi 62102, Taiwan

⁶Division of Dentistry, Kaohsiung Armed Forces General Hospital, 2, Zhongzheng 1st. Rd., Kaohsiung City 80284, Taiwan

⁷Director of Technology Development, Hitspectra Intelligent Technology Co., Ltd., 4F, No.2, Fuxing 4th Rd., Qianzhen District, Kaohsiung 80661, Taiwan

⁸Department of Medical Research, Dalin Tzu Chi Hospital, Buddhist Tzu Chi Medical Foundation, No. 2, Minsheng Road, Dalin, Chiayi 62247, Taiwan

Abstract:

Background: Dental implants are critical for restoring functionality and aesthetics in patients with missing teeth. The all-on-four treatment concept utilizes four dental implants to support a full-arch prosthesis. Material choice for these implants plays a crucial role in the long-term success of the treatment, affecting everything from biomechanical stability to osseointegration and patient comfort.

Aim: The purpose of this study is to analyze the biomechanical performance of three different materials used in all-on-four dental implant designs through finite element analysis (FEA). The aim is to determine which material optimally balances stress and deformation under various loading conditions.

Objective: The main objective of this research is to evaluate the effects of stress, strain, and deformation on all-on-four dental implants made from titanium, zirconia, and polyether ether ketone (PEEK). The study seeks to identify which material demonstrates the best mechanical properties under simulated functional loads.

Methods: A 3D model simulating the dental implants integrated with cancellous and cortical bone was developed. Finite element analysis was conducted to assess the biomechanical performance of the implants made from titanium, zirconia, and PEEK. A perpendicular load of 100 N was applied to the tips of the implants, followed by an oblique load of 100 N at a 30-degree angle, to simulate different chewing forces.

Results: The deformation analysis indicated that implants made of zirconia exhibited significantly lower maximum and average deformation compared to those made from titanium and PEEK. Although PEEK implants showed lower maximum and average stress, they did not perform well in stress dissipation compared to zirconia. Similar patterns of stress and deformation were observed under both perpendicular and oblique loading conditions.

Conclusion: Zirconia implants outperformed titanium and PEEK in terms of deformation and stress distribution under simulated loading conditions. This suggests that zirconia could be a superior material for all-on-four dental implants, offering better mechanical stability and potentially enhancing the longevity and success of dental restorations. Further clinical trials are recommended to validate these findings and assess the long-term outcomes of zirconia-based implants.

Keywords: Dental Implants, FEA analysis, All-on-four, Deformation, Stress, Strain, PEEK, Zirconia, Titanium.

© 2024 The Author(s). Published by Bentham Open.

This is an open access article distributed under the terms of the Creative Commons Attribution 4.0 International Public License (CC-BY 4.0), a copy of which is available at: <https://creativecommons.org/licenses/by/4.0/legalcode>. This license permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.



Received: May 10, 2024
Revised: June 07, 2024
Accepted: June 07, 2024
Published: ?? ??, 2024



Send Orders for Reprints to
reprints@benthamscience.net

*Address correspondence to these authors at the Department of Mechanical Engineering, National Chung Cheng University, 168, University Rd., Min Hsiung, Chia Yi 62102, Taiwan, Director of Technology Development, HITSPECTRA Intelligent Technology Co., Ltd., 4F, No.2, Fuxing 4th Rd., Qianzhen District, Kaohsiung 80661, Taiwan, Department of Medical Research, Dalin Tzu Chi Hospital, Buddhist Tzu Chi Medical Foundation, No. 2, Minsheng Road, Dalin, Chiayi, 62247 Taiwan and Division of Dentistry, Kaohsiung Armed Forces General Hospital, 2, Zhongzheng 1st. Rd., Kaohsiung City 80284, Taiwan; E-mails: m97510051225@gmail.com and hcwang@ccu.edu.tw

#These authors contributed equally to this work.

Cite as: Chang C, Karmakar R, Mukundan A, Lu S, Choomjinda U, Chen M, Chen Y, Wang H. Mechanical Integrity of All-on-Four Dental Implant Systems: Finite Element Simulation of Material Properties of Zirconia, Titanium, and PEEK. *Open Dent J*, 2024; 18: e18742106325708. <http://dx.doi.org/10.2174/0118742106325708240614044708>

1. INTRODUCTION

Many techniques have been used to monitor the performance of dental implants. One such method is hyperspectral imaging (HSI) where a spectrometer can be used to detect the biofilm contaminations on dental implants [1, 2]. Specifically, with the improvement in snapshot-based HSI, which has been used in many other medical and other applications, dental implant performance analysis in the future will be much more convenient [3-9]. In recent years, many types of biosensors have also been developed [10-12]. One study that used a micro bio-sensor built inside the dental implant has already been proposed [13]. However, there are few studies on these methods, and all these methods can only be used after the dental implant has been fixed. Finite element analysis (FEA) has long been used to measure the effects of stress-strain and deformation in dental implants [14, 15]. In particular, the effectiveness of any dental implant is reliant on a wide range of variables that influence bone-implant, implant-abutment, and abutment-prosthesis integrations [16, 17]. Examining the force distribution, including the stress-strain and deformation values, is essential in determining the success of any implant [18, 19]. One of the latest designs to overcome general failures is known as the "all-on-four" configuration, which uses only four implants, namely, two in the anterior region and two in the posterior region [20-22]. Many studies have performed FEA on all-on-four designs and proven its feasibility [23-27].

Another factor affecting the success of a dental impact is its material. Since the early 1960s, titanium has been used as a primary material for dental implants because of its economic viability, biocompatibility, extensive human clinical success, and bone bonding capacity [28-30]. Owing to aesthetics, many ceramic-based implants have been investigated in recent years [31, 32]. One such material is zirconia [33, 34]. Zirconia offers great resistance to oxidation, higher wear resistance, a high Weibull modulus, excellent flexural modulus, fracture toughness, and static fracture strength [35]. In addition, zirconia has a low thermal conductivity [36]. Although zirconia has exceptional short-term results, high-quality long-term studies are lacking [37]. Polyether ether ketone (PEEK) is a metal-free biocompatible thermoplastic polymer that is

also currently being used in dental implants [38, 39]. PEEK has excellent mechanical qualities, high-temperature resistance, chemical stability, strong wear resistance, and high bond strength [40, 41]. However, PEEK has a much lower modulus of elasticity and low hardness [42, 43]. Comprehensive studies involving PEEK are also rare [44].

In our previous study, the effects of increasing the number of fences to support dental implants were investigated [45]. According to the results of the FEA analysis, 74% of the deformation and 80% of the stress occurred when the number of fences was increased from one to three. In general, as the number of fences increases, the stress dissipation results are enhanced. However, only titanium as a material for dental implants was considered in the study. In the current study, PEEK, zirconia, and titanium all-on-four dental implants were subject to a 100 N perpendicular load on four tips of dental implants. Then, the effects of stress-strain and deformation were investigated. An oblique load of 100 N at 30° was also applied, and comparative results were examined.

2. MATERIALS AND METHODS

2.1. Software

PEEK, zirconia, and titanium materials were compared for their deformation and strain-stress results. Dassault Systemes' CATIA version 6 was utilized to construct the 3D model. The Finite Element Analysis (FEA) was conducted using Ansys version 2021 R2. The chosen design was simplified within limits that would not disrupt the local stress analysis, considering the intricate geometries of jawbones. The implemented design provides a foundation for conducting a comparative evaluation of three distinct materials and their corresponding deformation and strain-stress solutions, as derived from analytical investigations.

2.2. Design and FEA

The implant had a diameter of 4.5 mm and a total length of 8 mm. The radius of the bottom two fences was 2 mm, and the top fence had a diameter of 1.5 mm, following the configuration in our previous study 45. Given the dramatic shift in stress at the edges, the junctures

3. RESULTS

3.1. Deformation

The deformation results of the three materials are shown in Table 2, while Fig. (1) shows a comparison of the deformation results. A force of 100 N at the four tips of the dental implants was applied, totaling 400 N. The deformation results showed that zirconia had the lowest maximum deformation of 1.2673 μm , followed by titanium at 1.7449 μm . PEEK had the highest maximum deformation of 8.4035 μm . Although the maximum deformation results of titanium and zirconia were similar, the average deformation of the latter was much lower at 0.197 μm (titanium: 1.4594 μm). The obtained values indicate that zirconia was suitable for the three-fenced all-on-four implants and dissipated the deformation better than PEEK and titanium. Compared with the results of PEEK, the maximum total deformation of zirconia was reduced by 84.91% and compared with the results of titanium, the maximum total deformation of zirconia was reduced by 27.37%. This slight reduction in deformation over the years can increase the performance of the dental implant.

3.2. Stress

The results of the stress analysis (maximum, minimum, and average stresses) at 100 N for each tip of the dental implants for all three materials are shown in Table 3. A visual representation of the same results is shown in Fig. (2). The results showed that PEEK had the lowest

maximum stress of 8.9674 MPa, whereas the highest maximum stress was for zirconia at 15.466 MPa. Titanium obtained a moderate maximum stress of 13.507 MPa. An interesting result was observed for the average stress. In particular, zirconia had the best average stress of 0.46083 MPa, whereas titanium and PEEK had average stresses of 4.5025 and 4.5528 MPa, respectively. The simulation results of the average stress indicate that although the maximum stress of zirconia is higher, its stress dissipation is much more efficient. The maximum stress of PEEK was much lower, while its average stress was much higher, indicating its poor stress dissipation capability. Effective stress dissipation can be calculated by comparing the average stress with the maximum stress. Here, PEEK had the poorest stress dissipation at 49.22%, whereas titanium had a better measure of 66.65%. Zirconia had the best stress dissipation measure at 97.0224%. These values indicate that zirconia can efficiently dissipate most of the stress.

3.3. Strain

The results of the strain analysis are shown in Table 4, in which a force of 100 N perpendicular to the dental implant was applied at the four tips. Fig. (3) shows the result of the strain analysis. Overall, the results of the strain analysis were similar to those of the stress analysis. Although PEEK had a lower strain, its average strain was much higher than those of zirconia and titanium. Although zirconia had a much higher strain rate, its average strain was the lowest among the three materials. Titanium had a moderate maximum strain and average strain.

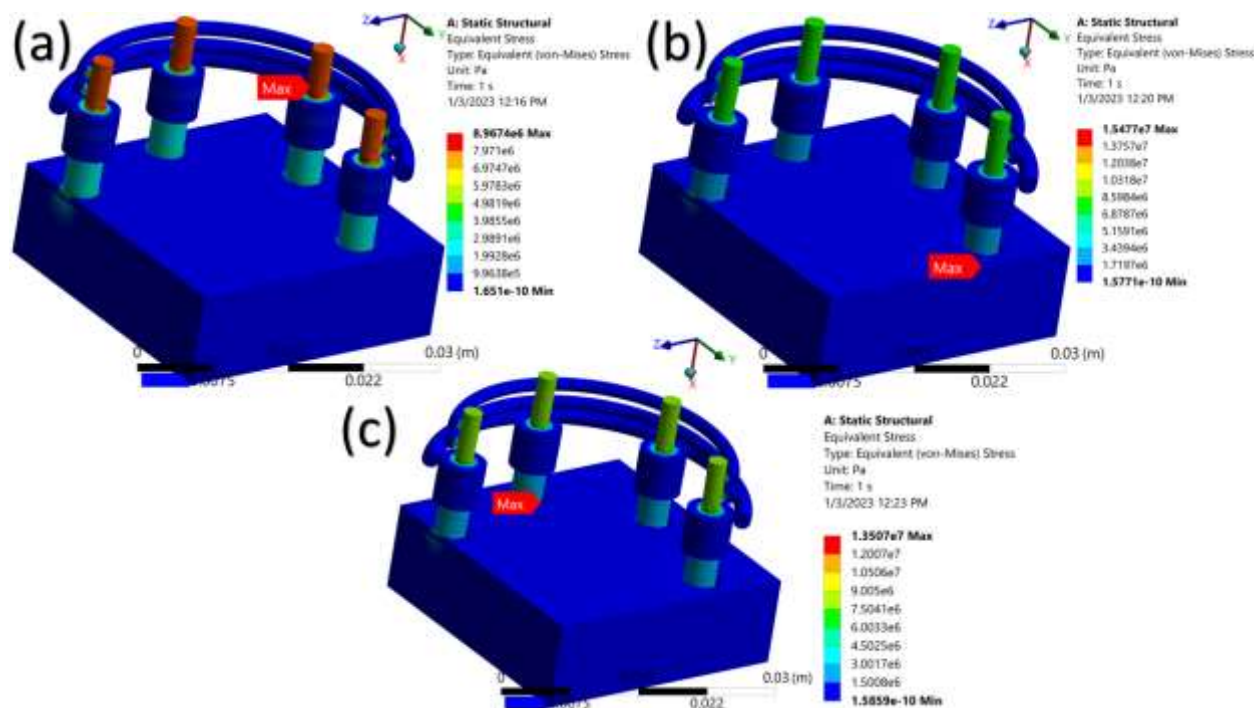


Fig. (2). Equivalent von Mises stress of the three different materials. (a-c) PEEK, zirconia, and titanium materials, respectively.

Table 3. Minimum, maximum, and average stress results of the titanium, zirconia, and PEEK materials.

Material	Minimum Stress (MPa)	Maximum Stress (MPa)	Average Stress (MPa)
Titanium	1.5899×10^{-16}	13.507	4.5025
Zirconia	1.5772×10^{-16}	15.477	0.46083
PEEK	3.6469×10^{-16}	8.9674	4.5528

Table 4. Minimum, maximum, and average strain results of the titanium, zirconia, and PEEK materials.

Material	Minimum Strain	Maximum Strain	Average Strain
Titanium	2.2346×10^{-21}	2.9244×10^{-3}	3.2493×10^{-5}
Zirconia	2.2205×10^{-21}	2.986×10^{-3}	8.9055×10^{-6}
PEEK	2.3261×10^{-21}	2.6274×10^{-3}	4.1713×10^{-5}

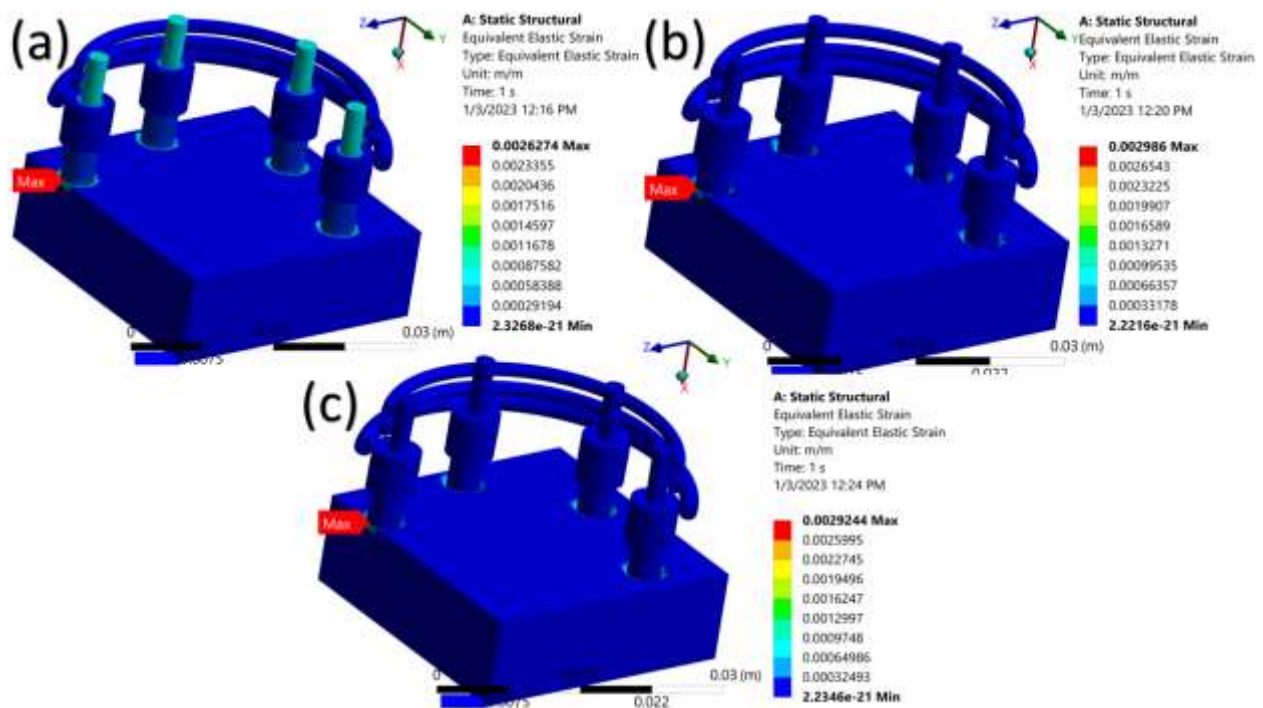


Fig. (3). Equivalent von Mises strain of three different materials at a 30-degree oblique load of 100 N. (a-c) show titanium, zirconia, and PEEK materials, respectively.

3.4. Oblique Loading Analysis

Another factor considered in the FEA of dental implants is the process of mastication, also known as chewing. Here, the effect of an oblique load of 100 N, each at 30° on the four tips of the implant, was investigated. The deformation results of the oblique load of all three materials are shown in Table 5. A visual representation of the results is shown in Fig. (4). Overall, the results indicate that zirconia had a much lower maximum deformation and a lower average deformation, PEEK had the highest maximum deformation and a higher average deformation, and titanium performed reasonably.

The stress results of applying the oblique load on all three materials are shown in Table 6, and a visual representation of the results is shown in Fig. (5). The stress results of applying an oblique load of 100 N at 30° were similar to those under a perpendicular load. Zirconia had the maximum stress, whereas PEEK had a much lower stress value. The average stress of zirconia was much lower at 5.7217 MPa, whereas that of PEEK was 4.5 MPa. The stress dissipation of zirconia was 99.0644%, whereas that of PEEK was 98.1926%. The stress dissipation ratio of titanium was 98.805%. The maximum stress and average stress values were much lower for PEEK, whereas the stress dissipation measure was higher for zirconia.

Table 5. Total deformation results of the three different materials at a 30-degree oblique load of 100 N.

Material	Minimum Deformation (µm)	Maximum Deformation (mm)	Average Deformation (µm)
Titanium	0	0.27742	18.494
Zirconia	0	0.20841	14.43
PEEK	0	0.93911	45.893

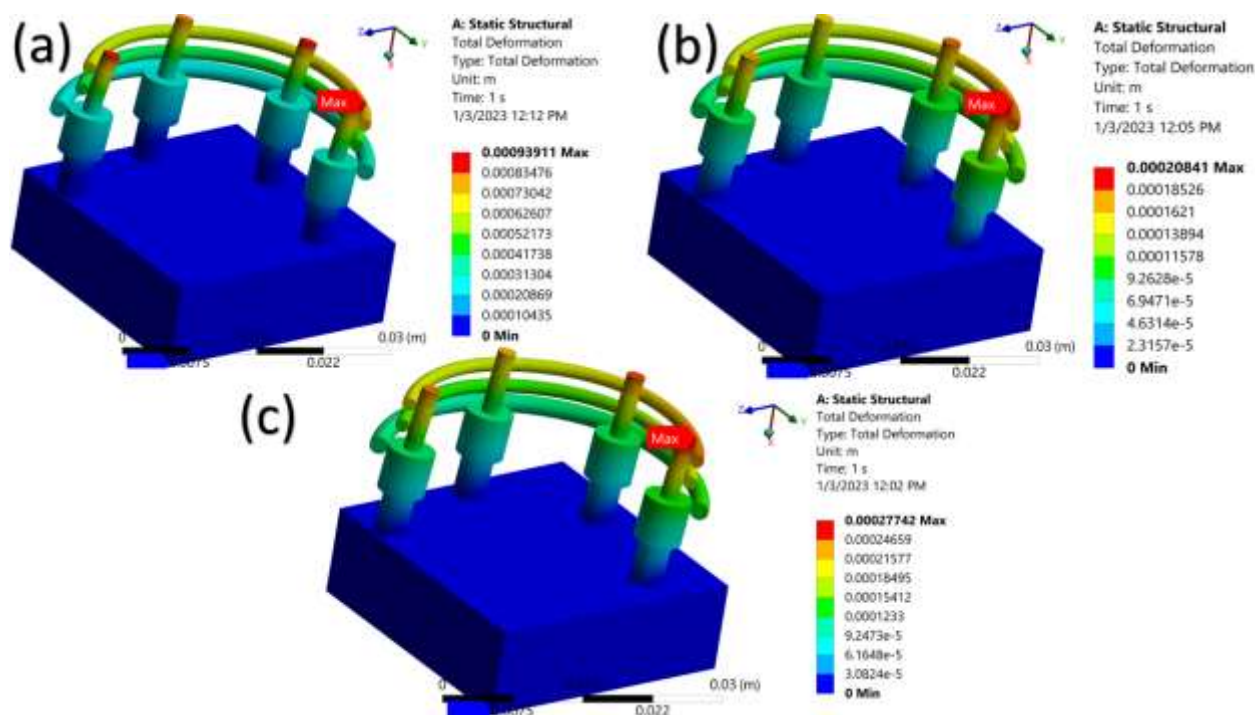


Fig. (4). Total deformation of the three different materials at an oblique load of 30° of 100 N. (a-c) PEEK, zirconia, and titanium materials, respectively.

4. DISCUSSION

In this study, the FEA of three-fenced all-on-four dental implants was investigated based on three materials, namely, titanium, zirconia, and PEEK. The stress-strain and deformation results for a perpendicular load of 100 N applied at the four tips of the dental implant were obtained. An oblique load of 100 N at 30° was also applied on the four tips of the dental implant, and similar results were obtained. The deformation results showed that zirconia had less deformation than PEEK and titanium. However, the stress analysis showed that PEEK had a much lower maximum stress and average stress. The

stress dissipation measure also showed that zirconia was much better at dissipating the stress to the surrounding fences.

Furthermore, deformation analysis showed that the maximum deformation was located at the tip of the dental implant, and a large amount of stress was found at the fences. Most of the higher stress for PEEK was found on the dental implant, whereas the maximum deformations for titanium and zirconia were found at the interjunction of the dental implant with the bone. The deformation of PEEK can cause an earlier failure of the dental implant because of the highly concentrated stress on the dental implants (Supplementary Material).

Table 6. Equivalent von Mises stress results of the three different materials at a 30-degree oblique load of 100 N.

Material	Minimum Stress (MPa)	Maximum Stress (MPa)	Average Stress (MPa)
Titanium	3.4808×10 ⁻¹⁶	422.6	5.048
Zirconia	1.5772E-10	611.56	5.7217
PEEK	3.6469E-10	248.99	4.5

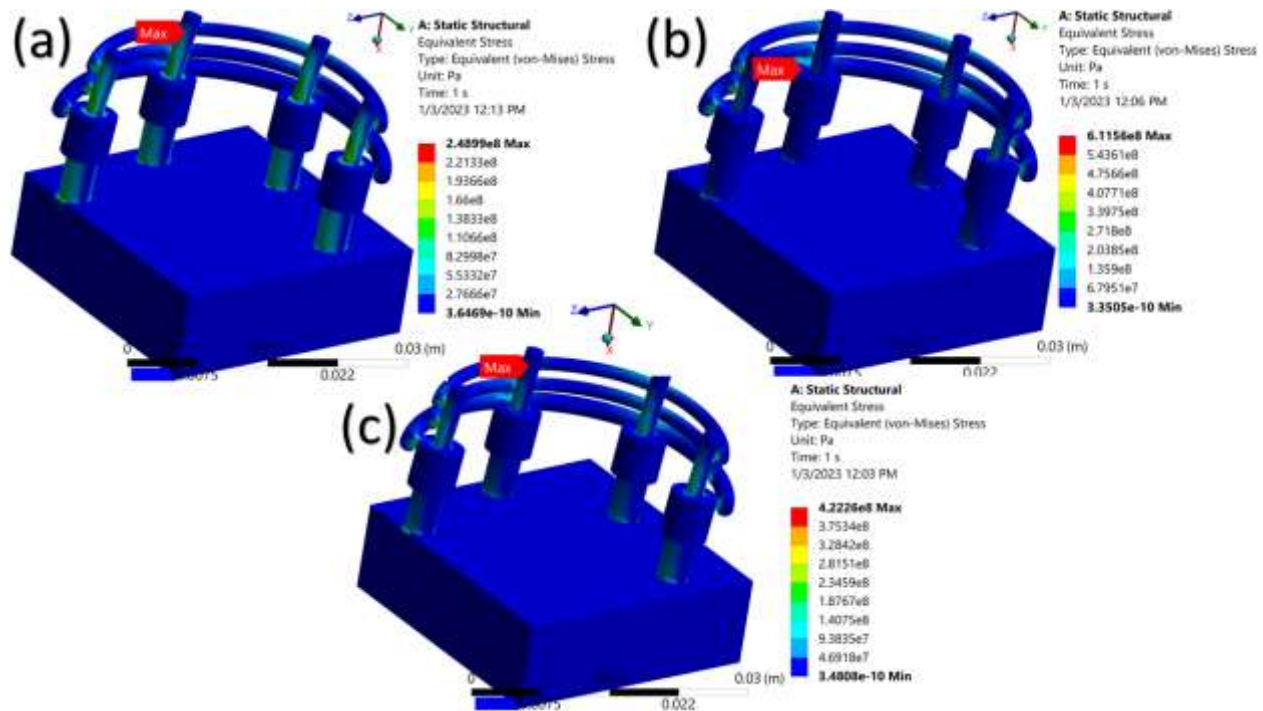


Fig. (5). Equivalent von Mises stress of three different materials at a 30-degree oblique load of 100 N. **(a, b and c)** PEEK, zirconia, and titanium materials, respectively.

CONCLUSION

Titanium, zirconia, and PEEK materials were evaluated by FEA for a three-fenced all-on-four dental implant in this study. The stress-strain and deformation for a perpendicular load of 100 N applied at each of the four tips of the dental implant were studied. In addition, an oblique load of 100 N at 30° was applied on each of the four tips of the dental implant, and the same results were obtained. The results of the deformation test indicate that zirconia had a lower degree of deformation than PEEK and titanium. The stress study, on the other hand, revealed that PEEK had a significantly lower maximum stress and a significantly lower average stress. On the other hand, the stress dissipation result demonstrated that zirconia was significantly more effective for transferring stress to the fences in the surrounding area.

AUTHORS' CONTRIBUTION

Conceptualization, C.-L.C., H.-C.W., and A.M. ; data curation, C.-L.C, R.K., and A.M. ; formal analysis, C.-L.C., R.K., and A.M. ; funding acquisition, R.K., A.M., and H.-C.W. ; investigation, S.-H.L., and A.M. ; methodology, S.-H.L, H.-C.W., U.C., and A.M. ; project administration, S.-H.L., U.C., and H.-C.W. ; resources, U.C., S.-H.L., M.-M.C., and H.-C.W. ; software, M.-M.C., S.-C.C., and A.M. ; supervision, Y.-L.C., and H.-C.W. ; validation, Y.-L.C., H.-C.W., and A.M. ; writing—original draft, Y.-L.C and A.M. ; writing—review and editing, A.M. and H.-C.W. All authors have read and agreed to the published version of the manuscript.

LIST OF ABBREVIATIONS

FEA = Finite Element Analysis
PEEK = Polyether Ether Ketone

ETHICS APPROVAL AND CONSENT TO PARTICIPATE

Not applicable.

HUMAN AND ANIMAL RIGHTS

Not applicable.

CONSENT FOR PUBLICATION

Not applicable.

AVAILABILITY OF DATA AND MATERIALS

The data supporting the findings of the article is available in the Open Dentistry Taiwan at https://www.myqnapcloud.com/share/745418i47p84o221384v25ad_336d7h7jk33m2491q16www6ayab7cf6k?session_id=2%7C1%3A0%7C10%3A1718938481%7C19%3Aession_portal_got_o%7C48%3AOTVmNzg2MWUtZDUwOS00YjhhLTjOGYtMGlzYTE3YWY3Mzk3%7C5caad005561ad352791edd227185f33d112d7eb8f4f63b07fcde6dabe82472cd#/home, reference as Den_pap_Supplement. All figures and tables are produced by authors.

FUNDING

This research was supported by the National Science and Technology Council, the Republic of China (Taiwan)

under grants NSTC 112-2221-E-194-036 and 112-2634-F-194-001. This work was financially/partially supported by the Kaohsiung Armed Forces General Hospital research project KAFGH_D_113030, and the Dalin Tzu Chi Hospital, Buddhist Tzu Chi Medical Foundation-National Chung Cheng University Joint Research Program in Taiwan.

CONFLICT OF INTEREST

The authors declare no conflict of interest, financial or otherwise.

ACKNOWLEDGEMENTS

Declared none.

SUPPLEMENTARY MATERIALS

The following supporting information can be downloaded at https://www.myqnapcloud.com/share/745418i47p84o221384v25ad_336d7h7jk33m2491q16www6ayab7cf6k?session_id=2%7C1%3A0%7C10%3A1718938481%7C19%3Asession_portal_goto%7C48%3AOTVmNzg2MWUtZDUwOS00YjhhLThjOGYtMGlyYTE3YWY3Mzk3%7C5caad005561ad352791edd227185f33d112d7eb8f4f63b07fcd6dabe82472cd#/home, Video S1. Total Deformation of PEEK at a perpendicular force of 100 N, Video S2. Total Deformation of PEEK at an angular force of 100 N, Video S3. Equivalent Elastic Strain of PEEK at a perpendicular force of 100 N, Video S4. Equivalent Elastic Strain of PEEK at an angular force of 100 N, Video S5. Equivalent Elastic Stress of PEEK at a perpendicular force of 100 N, Video S6. Equivalent Elastic Stress of PEEK at an angular force of 100 N, Video S7. Total deformation of zirconia at a perpendicular force of 100 N, Video S8. Total Deformation of Zirconia at an angular force of 100 N, Video S9. Equivalent Elastic Strain of Zirconia at a perpendicular force of 100 N, Video S10. Equivalent Elastic Strain of Zirconia at an angular force of 100 N, Video S11. Equivalent Elastic Stress of Zirconia at a perpendicular force of 100 N, Video S12. Equivalent Elastic Stress of Zirconia at an angular force of 100 N, Video S13. Total Deformation of Titanium at a perpendicular force of 100 N, Video S14. Total Deformation of Titanium at an angular force of 100 N, Video S15. Equivalent Elastic Strain of Titanium at a perpendicular force of 100 N, Video S16. Equivalent Elastic Strain of Titanium at an angular force of 100 N, Video S17. Equivalent Elastic Stress of Titanium at a perpendicular force of 100 N, Video S18. Equivalent elastic stress of titanium at an angular force of 100 N.

REFERENCES

- [1] Benic GI, Elmasry M, Hämmerle CHF. Novel digital imaging techniques to assess the outcome in oral rehabilitation with dental implants: A narrative review. *Clin Oral Implants Res* 2015; 26(S11) (Suppl. 11): 86-96. <http://dx.doi.org/10.1111/clr.12616> PMID: 26010421
- [2] Kim D-H, Kim MS, Hwang J. Monitoring of biofilm formation on different material surfaces of medical devices using hyperspectral imaging method. *Proceedings of SPIE* 2012; 27-33. <http://dx.doi.org/10.1117/12.909980>
- [3] Huang SY, Mukundan A, Tsao YM, Kim Y, Lin FC, Wang HC. Recent advances in counterfeit art, document, photo, hologram, and currency detection using hyperspectral imaging. *Sensors*

- 2022; 22(19): 7308. <http://dx.doi.org/10.3390/s22197308> PMID: 36236407
- [4] Mukundan A, Tsao YM, Lin FC, Wang HC. Portable and low-cost hologram verification module using a snapshot-based hyperspectral imaging algorithm. *Sci Rep* 2022; 12(1): 18475. <http://dx.doi.org/10.1038/s41598-022-22424-5> PMID: 36323727
- [5] Tsai TJ, Mukundan A, Chi YS, *et al.* Intelligent identification of early esophageal cancer by band-selective hyperspectral imaging. *Cancers* 2022; 14(17): 4292. <http://dx.doi.org/10.3390/cancers14174292> PMID: 36077827
- [6] Fang YJ, Mukundan A, Tsao YM, Huang CW, Wang HC. Identification of early esophageal cancer by semantic segmentation. *J Pers Med* 2022; 12(8): 1204. <http://dx.doi.org/10.3390/jpm12081204> PMID: 35893299
- [7] Tsai TJ, Mukundan A, Chung CS, *et al.* Hyperspectral imaging combined with artificial intelligence in the early detection of esophageal cancer. *Cancers (Basel)* 2021; 13(18): 4593. <http://dx.doi.org/10.3390/cancers13184593> PMID: 34572819
- [8] Chen CW, Tseng YS, Mukundan A, Wang HC. Air pollution: Sensitive detection of PM2.5 and PM10 concentration using hyperspectral imaging. *Appl Sci* 2021; 11(10): 4543. <http://dx.doi.org/10.3390/app11104543>
- [9] Mukundan A, Huang CC, Men TC, Lin FC, Wang HC. Air pollution detection using a novel snap-shot hyperspectral imaging technique. *Sensors* 2022; 22(16): 6231. <http://dx.doi.org/10.3390/s22166231> PMID: 36015992
- [10] Mukundan A, Feng SW, Weng YH, *et al.* Optical and material characteristics of MoS₂/Cu₂O sensor for detection of lung cancer cell types in hydroplegia. *Int J Mol Sci* 2022; 23(9): 4745. <http://dx.doi.org/10.3390/ijms23094745> PMID: 35563136
- [11] Mukundan A, Tsao YM, Artemkina SB, Fedorov VE, Wang HC. Growth mechanism of periodic-structured MoS₂ by transmission electron microscopy. *Nanomaterials* 2021; 12(1): 135. <http://dx.doi.org/10.3390/nano12010135> PMID: 35010085
- [12] Hsiao YP, Mukundan A, Chen WC, Wu MT, Hsieh SC, Wang HC. Design of a lab-on-chip for cancer cell detection through impedance and photoelectrochemical response analysis. *Biosensors (Basel)* 2022; 12(6): 405. <http://dx.doi.org/10.3390/bios12060405> PMID: 35735553
- [13] Li YJ, Lu CC. A novel scheme and evaluations on a long-term and continuous biosensor platform integrated with a dental implant fixture and its prosthetic abutment. *Sensors* 2015; 15(10): 24961-76. <http://dx.doi.org/10.3390/s151024961> PMID: 26404283
- [14] Chun HJ, Cheong SY, Han JH, *et al.* Evaluation of design parameters of osseointegrated dental implants using finite element analysis. *J Oral Rehabil* 2002; 29(6): 565-74. <http://dx.doi.org/10.1046/j.1365-2842.2002.00891.x> PMID: 12071926
- [15] Van Staden RC, Guan H, Loo YC. Application of the finite element method in dental implant research. *Comput Methods Biomech Biomed Engin* 2006; 9(4): 257-70. <http://dx.doi.org/10.1080/10255840600837074> PMID: 17132532
- [16] Geng JP, Tan KBC, Liu GR. Application of finite element analysis in implant dentistry: A review of the literature. *J Prosthet Dent* 2001; 85(6): 585-98. <http://dx.doi.org/10.1067/mps.2001.115251> PMID: 11404759
- [17] Kayabaşı O, Yüzbasioğlu E, Erzincanlı F. Static, dynamic and fatigue behaviors of dental implant using finite element method. *Adv Eng Softw* 2006; 37(10): 649-58. <http://dx.doi.org/10.1016/j.advengsoft.2006.02.004>
- [18] Vaillancourt H, Pilliar RM, McCammond D. Factors affecting crestal bone loss with dental implants partially covered with a porous coating: A finite element analysis. *Int J Oral Maxillofac Implants* 1996; 11(3): 351-9. PMID: 8752556
- [19] Pilliar RM, Deporter DA, Watson PA, Valiquette N. Dental implant design-effect on bone remodeling. *J Biomed Mater Res* 1991; 25(4): 467-83.

- <http://dx.doi.org/10.1002/jbm.820250405> PMID: 2050711
- [20] Maló P, Rangert B, Dvårsäter L. Immediate function of Brånemark implants in the esthetic zone: A retrospective clinical study with 6 months to 4 years of follow-up. *Clin Implant Dent Relat Res* 2000; 2(3): 138-46.
<http://dx.doi.org/10.1111/j.1708-8208.2000.tb00004.x> PMID: 11359258
- [21] Maló P, Friberg B, Polizzi G, Gualini F, Vighagen T, Rangert B. Immediate and early function of Brånemark System implants placed in the esthetic zone: A 1-year prospective clinical multicenter study. *Clin Implant Dent Relat Res* 2003; 5(s1) (Suppl. 1): 37-46.
<http://dx.doi.org/10.1111/j.1708-8208.2003.tb00014.x> PMID: 12691649
- [22] Maló P, Rangert B, Nobre M. "All-on-Four" immediate-function concept with Brånemark System implants for completely edentulous mandibles: A retrospective clinical study. *Clin Implant Dent Relat Res* 2003; 5(s1) (Suppl. 1): 2-9.
<http://dx.doi.org/10.1111/j.1708-8208.2003.tb00010.x> PMID: 12691645
- [23] Saleh Saber F, Ghasemi S, Koodaryan R, Babaloo A, Abolfazli N. The comparison of stress distribution with different implant numbers and inclination angles in all-on-four and conventional methods in maxilla: A finite element analysis. *J Dent Res Dent Clin Dent Prospect* 2015; 9(4): 246-53.
<http://dx.doi.org/10.15171/joddd.2015.044> PMID: 26889362
- [24] Silva GC, Mendonça JA, Lopes LR, Landre J Jr. Stress patterns on implants in prostheses supported by four or six implants: A three-dimensional finite element analysis. *Int J Oral Maxillofac Implants* 2010; 25(2): 239-46.
PMID: 20369081
- [25] Özdemir Doğan D, Polat NT, Polat S, Şeker E, Gül EB. Evaluation of "all-on-four" concept and alternative designs with 3D finite element analysis method. *Clin Implant Dent Relat Res* 2014; 16(4): 501-10.
<http://dx.doi.org/10.1111/cid.12024> PMID: 23217013
- [26] Liu T, Mu Z, Yu T, Wang C, Huang Y. Biomechanical comparison of implant inclinations and load times with the all-on-4 treatment concept: A three-dimensional finite element analysis. *Comput Methods Biomech Biomed Engin* 2019; 22(6): 585-94.
<http://dx.doi.org/10.1080/10255842.2019.1572120> PMID: 30821483
- [27] Ozan O, Kurtulmus-Yilmaz S. Biomechanical comparison of different implant inclinations and cantilever lengths in all-on-4 treatment concept by three-dimensional finite element analysis. *Int J Oral Maxillofac Implants* 2018; 33(1): 64-71.
<http://dx.doi.org/10.11607/jomi.6201> PMID: 29340344
- [28] Koizumi H, Takeuchi Y, Imai H, Kawai T, Yoneyama T. Application of titanium and titanium alloys to fixed dental prostheses. *J Prosthodont Res* 2019; 63(3): 266-70.
<http://dx.doi.org/10.1016/j.jpor.2019.04.011> PMID: 31147298
- [29] Nicholson W. Titanium alloys for dental implants: A review. *Prosthesis* 2020; 2: 11.
<http://dx.doi.org/10.3390/prosthesis2020011>
- [30] Hong DGK, Oh J. Recent advances in dental implants. *Maxillofac Plast Reconstr Surg* 2017; 39(1): 33.
<http://dx.doi.org/10.1186/s40902-017-0132-2> PMID: 29159171
- [31] Karapetian V, Sorg T, Jöckel M, Baumann M. Comparison of different polishing systems for dental inlay ceramics CAD/CAM in aesthetic dentistry. Chicago: Quintessence Publishing Co., Inc. 1996.
- [32] He LH, Swain M. A novel polymer infiltrated ceramic dental material. *Dent Mater* 2011; 27(6): 527-34.
<http://dx.doi.org/10.1016/j.dental.2011.02.002> PMID: 21371744
- [33] Pereira GKR, Guilardi LF, Dapieve KS, Kleverlaan CJ, Rippe MP, Valandro LF. Mechanical reliability, fatigue strength and survival analysis of new polycrystalline translucent zirconia ceramics for monolithic restorations. *J Mech Behav Biomed Mater* 2018; 85: 57-65.
<http://dx.doi.org/10.1016/j.jmbbm.2018.05.029> PMID: 29857261
- [34] Esquivel-Upshaw JF, Kim MJ, Hsu SM, *et al.* Randomized clinical study of wear of enamel antagonists against polished monolithic zirconia crowns. *J Dent* 2018; 68: 19-27.
<http://dx.doi.org/10.1016/j.jdent.2017.10.005> PMID: 29042241
- [35] Manicone PF, Rossi Iommetti P, Raffaelli L. An overview of zirconia ceramics: Basic properties and clinical applications. *J Dent* 2007; 35(11): 819-26.
<http://dx.doi.org/10.1016/j.jdent.2007.07.008> PMID: 17825465
- [36] Bankoğlu Güngör M, Aydın C, Yılmaz H, Gül EB. An overview of zirconia dental implants: Basic properties and clinical application of three cases. *J Oral Implantol* 2014; 40(4): 485-94.
<http://dx.doi.org/10.1563/AAID-JOI-D-12-00109> PMID: 25106014
- [37] Afrashtehfar KI, Del Fabbro M. Clinical performance of zirconia implants: A meta-review. *J Prosthet Dent* 2020; 123(3): 419-26.
<http://dx.doi.org/10.1016/j.prosdent.2019.05.017> PMID: 31451193
- [38] Bathala L, Majeti V, Rachuri N, Singh N, Gedela S. The role of polyether ether ketone (PEEK) in dentistry—a review. *J Med Life* 2019; 12(1): 5-9.
<http://dx.doi.org/10.25122/jml-2019-0003> PMID: 31123518
- [39] Skirbutis G, Dzingutė A, Masiliūnaitė V, Šulcaitė G, Žilinskas J. PEEK polymer's properties and its use in prosthodontics. A review. *Stomatologija* 2018; 20(2): 54-8.
PMID: 30531169
- [40] Wang H, Xu M, Zhang W, *et al.* Mechanical and biological characteristics of diamond-like carbon coated poly aryl-ether-ether-ketone. *Biomaterials* 2010; 31(32): 8181-7.
<http://dx.doi.org/10.1016/j.biomaterials.2010.07.054> PMID: 20692699
- [41] Wimmer T, Huffmann AMS, Eichberger M, Schmidlin PR, Stawarczyk B. Two-body wear rate of PEEK, CAD/CAM resin composite and PMMA: Effect of specimen geometries, antagonist materials and test set-up configuration. *Dent Mater* 2016; 32(6): e127-36.
<http://dx.doi.org/10.1016/j.dental.2016.03.005> PMID: 27033460
- [42] Moby V, Dupagne L, Fouquet V, Attal JP, François P, Dursun E. Mechanical Properties of Fused Deposition Modeling of Polyetheretherketone (PEEK) and interest for dental restorations: A systematic review. *Materials* 2022; 15(19): 6801.
<http://dx.doi.org/10.3390/ma15196801> PMID: 36234139
- [43] Papatheanasiou I, Kamposiora P, Papavasiliou G, Ferrari M. The use of PEEK in digital prosthodontics: A narrative review. *BMC Oral Health* 2020; 20(1): 217.
<http://dx.doi.org/10.1186/s12903-020-01202-7> PMID: 32741366
- [44] Porojan L, Toma FR, Vasiliu RD, Topală FI, Porojan SD, Maticescu A. Optical Properties and Color Stability of Dental PEEK related to artificial ageing and staining. *Polymers (Basel)* 2021; 13(23): 4102.
<http://dx.doi.org/10.3390/polym13234102> PMID: 34883606
- [45] Lee CH, Mukundan A, Chang SC, *et al.* Comparative analysis of stress and deformation between one-fenced and three-fenced dental implants using finite element analysis. *J Clin Med* 2021; 10(17): 3986.
<http://dx.doi.org/10.3390/jcm10173986> PMID: 34501431
- [46] Lekholm U, Zarb GA, Albrektsson T. Patient selection and preparation Tissue integrated prostheses. Chicago: Quintessence Publishing Co. Inc 1985; pp. 199-209.
- [47] Madfa AA, Al-Sanabani FA, Al-Qudami NH, Al-Sanabani JS, Amran AG. Use of zirconia in dentistry: An overview. *The Open Biomaterials Journal* 2014; 5: 1-9.
- [48] Kaleli N, Sarac D, Külünk S, Öztürk Ö. Effect of different restorative crown and customized abutment materials on stress distribution in single implants and peripheral bone: A three-dimensional finite element analysis study. *J Prosthet Dent* 2018; 119(3): 437-45.
<http://dx.doi.org/10.1016/j.prosdent.2017.03.008> PMID: 28645667
- [49] Xin H, Shepherd DET, Dearn KD. Strength of poly-ether-ether-ketone: Effects of sterilisation and thermal ageing. *Polym Test* 2013; 32(6): 1001-5.
<http://dx.doi.org/10.1016/j.polymertesting.2013.05.012>
- [50] Schwitalla A, Müller WD. PEEK dental implants: A review of the

- literature. *J Oral Implantol* 2013; 39(6): 743-9.
<http://dx.doi.org/10.1563/AAID-JOI-D-11-00002> PMID: 21905892
- [51] Guven S, Aguloglu S, Beydemir K, *et al.* Examination of stress distribution and fracture resistance in five-unit tooth- and implant-supported partial fixed zirconia prosthesis. *Biotechnol Biotechnol Equip* 2015; 29(6): 1176-83.
<http://dx.doi.org/10.1080/13102818.2015.1073122>
- [52] Niinomi M. Recent research and development in titanium alloys for biomedical applications and healthcare goods. *Sci Technol Adv Mater* 2003; 4(5): 445-54.
<http://dx.doi.org/10.1016/j.stam.2003.09.002>
- [53] Satoh T, Maeda Y, Komiyama Y. Biomechanical rationale for intentionally inclined implants in the posterior mandible using 3D finite element analysis. *Int J Oral Maxillofac Implants* 2005; 20(4): 533-9.
PMID: 16161737
- [54] Sevimay M, Turhan F, Kiliçarslan MA, Eskitascioglu G. Three-dimensional finite element analysis of the effect of different bone quality on stress distribution in an implant-supported crown. *J Prosthet Dent* 2005; 93(3): 227-34.
<http://dx.doi.org/10.1016/j.prosdent.2004.12.019> PMID: 15775923